


DO NOT ROTATE THE JEWELRY

STEP 1 (THE HEALING)

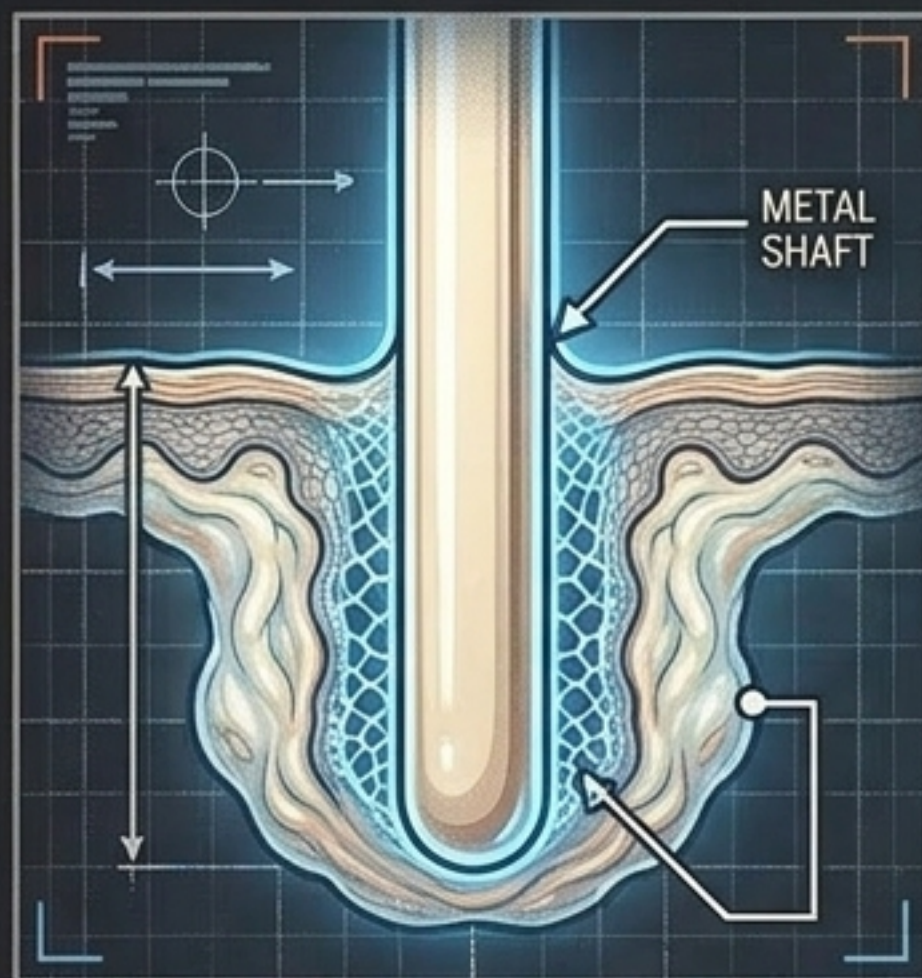

STEP 1 (THE HEALING)

Fragile new epithelial layer forms inside the fistula.

STEP 2 (THE ROTATION)



STEP 2 (THE ROTATION)

Movement physically tears the new cellular layer.

STEP 3 (THE CONTAMINATION)



STEP 3 (THE CONTAMINATION)

Rotation drags surface bacteria from the exposed jewelry directly into the deep wound channel.

Clean the exterior entry and exit points with sterile saline and leave the hardware alone.