THE HARDWARE VARIABLE

Reactive Alloy

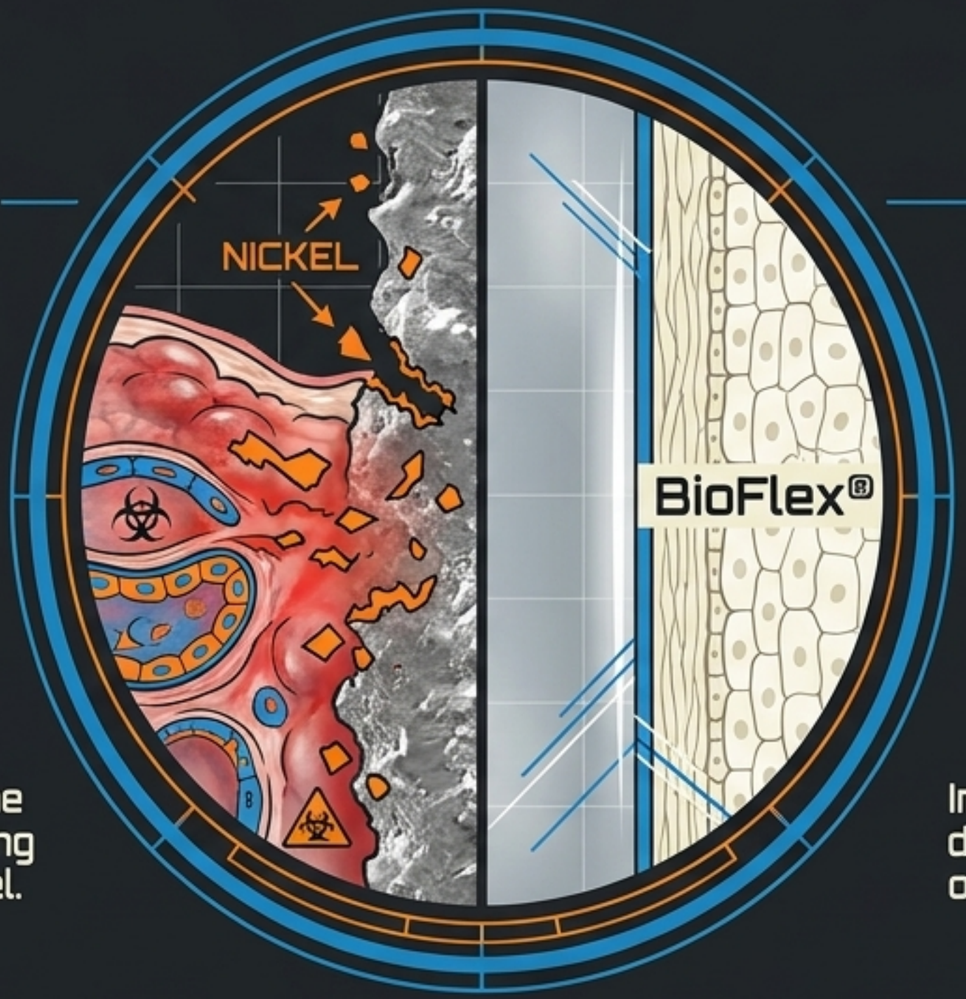

Medical Elastomer / Implant Grade

Unknown alloys degrade in the moist fistula, leaching sensitizing metals like nickel.

Implant-grade medical elastomers do not irritate maturing tracts or leach chemicals.

You cannot fix a bad jewelry choice with a good aftercare routine. The product and the hardware are two halves of the same equation.