


MEASURE TISSUE
FOLD DEPTH

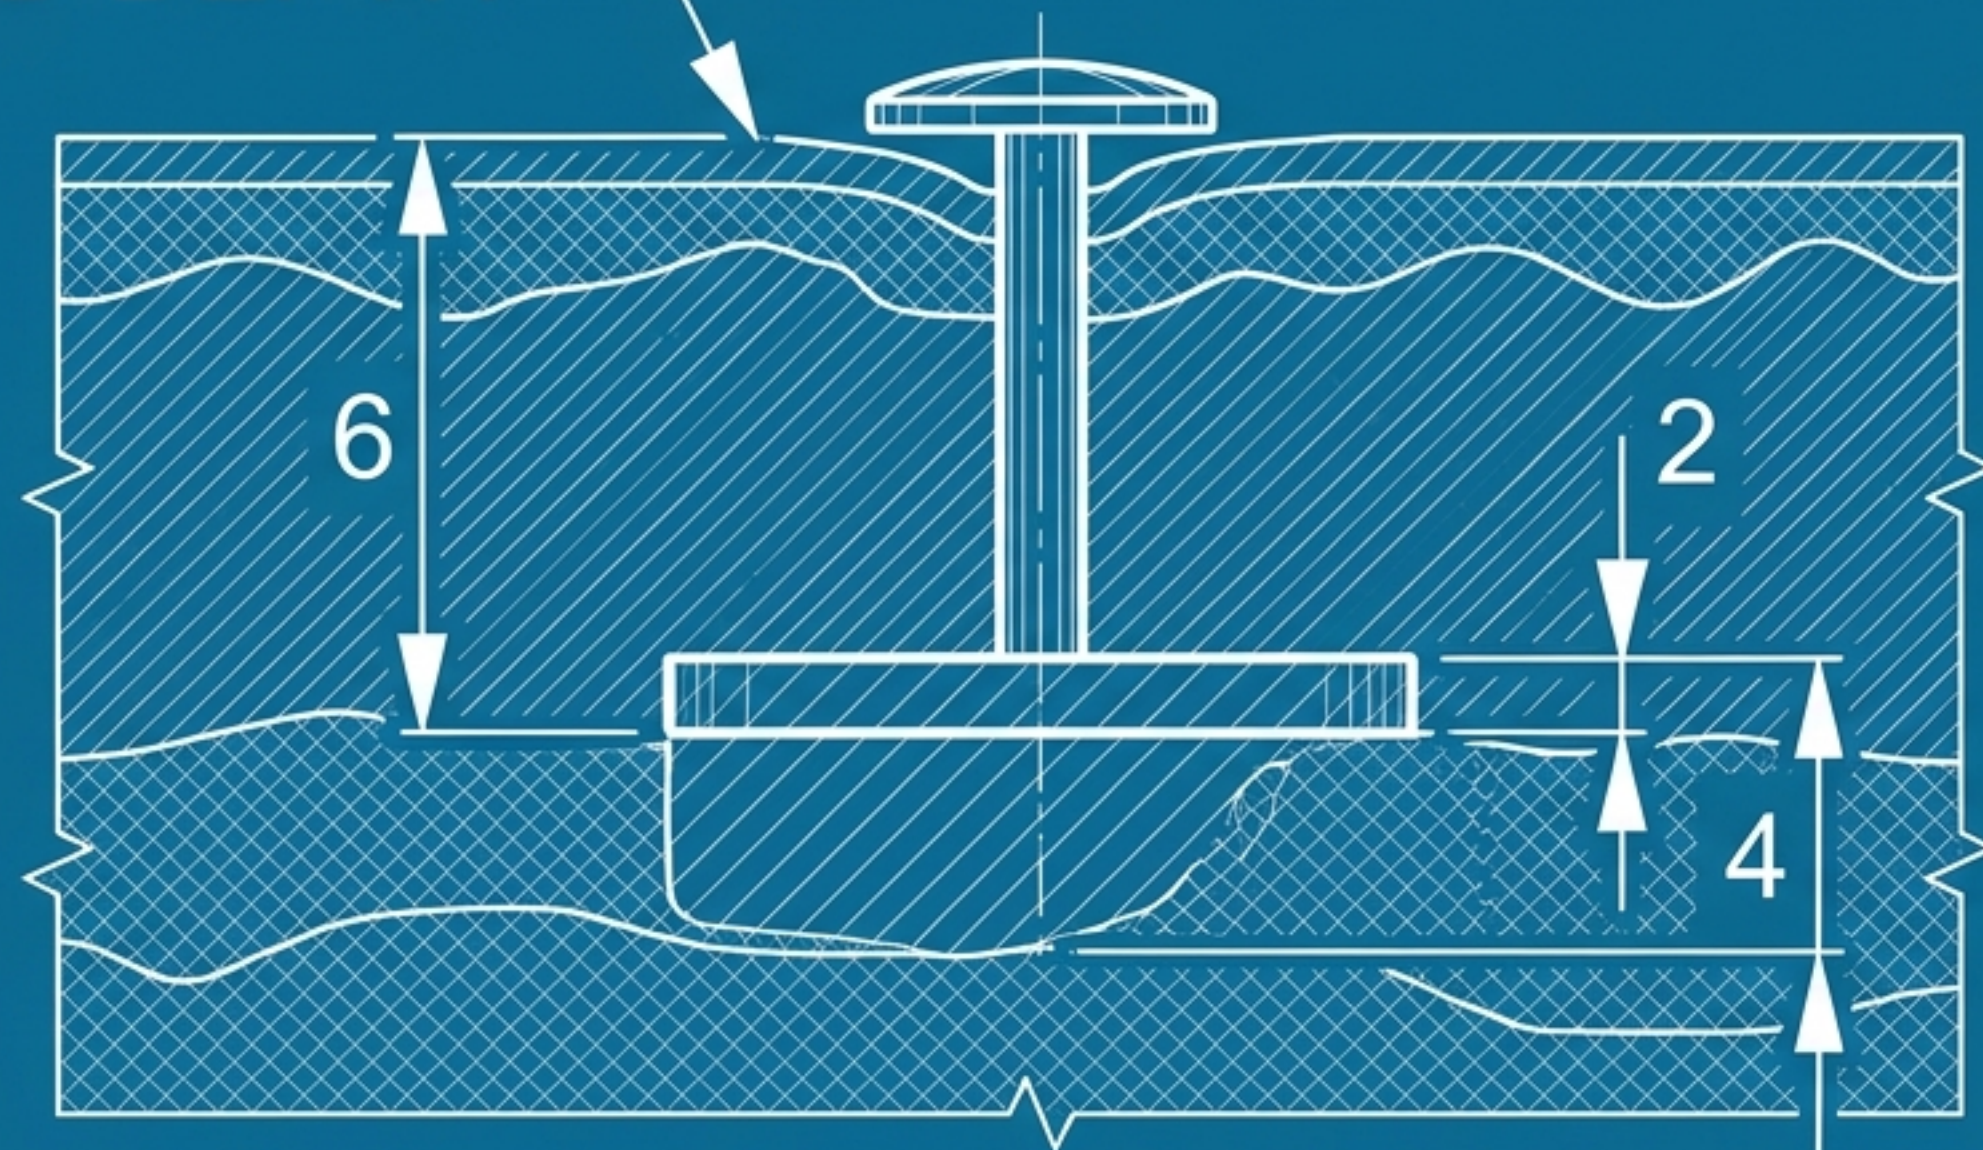

IMPLANT
SUB-DERMAL
LAYER

Minimum tissue depth between entry and exit points ensures stability.

VERIFY ALL PLACEMENT TOLERANCES