


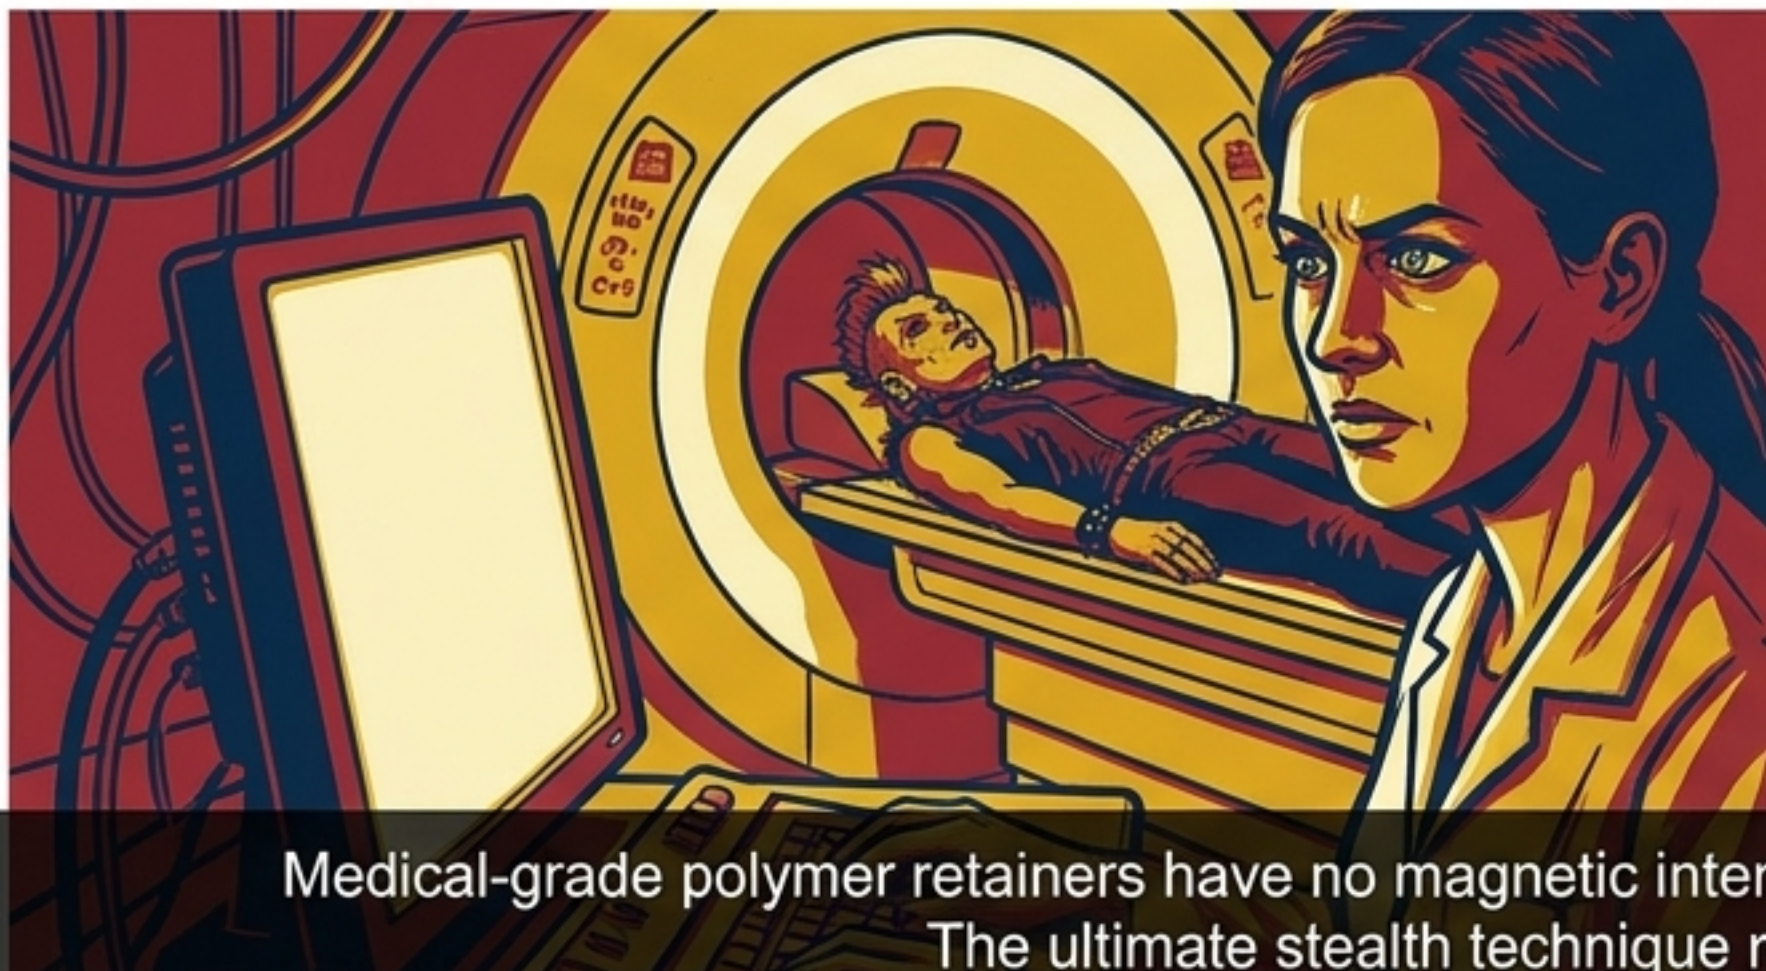

Medical-grade polymer retainers have no magnetic interaction and are entirely radiolucent on scanning equipment.
The ultimate stealth technique requires removing the heavy metal.