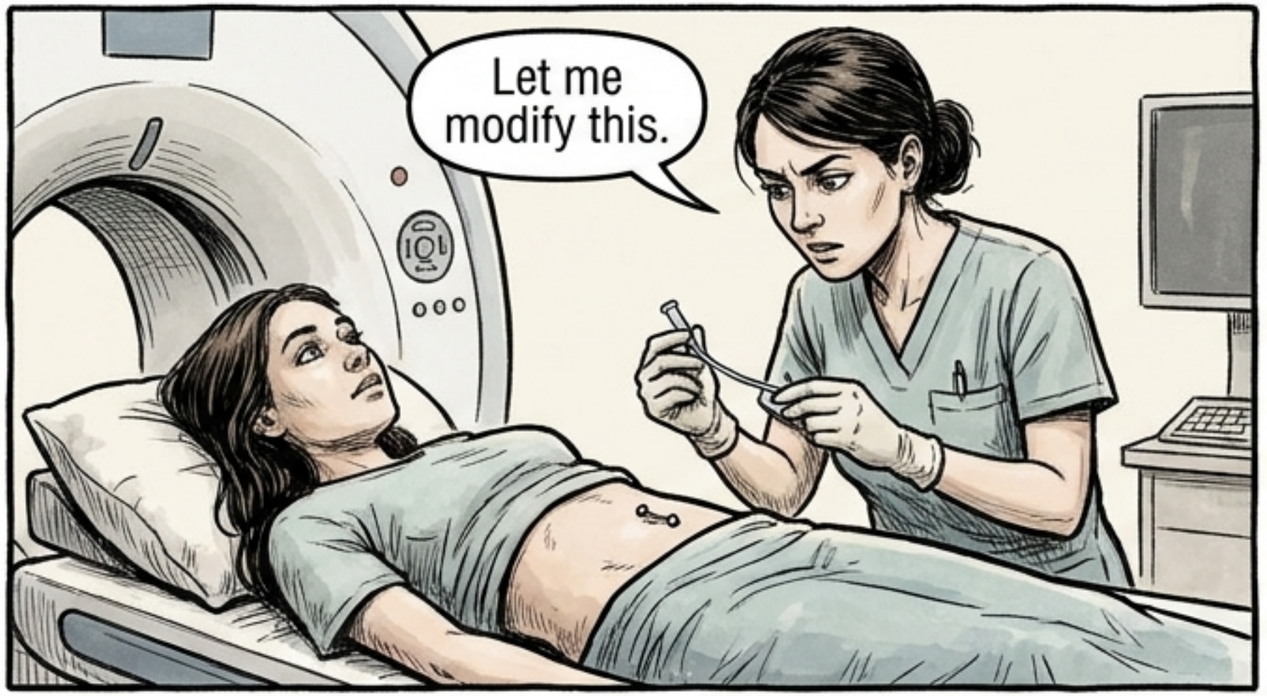

The plastic tube of an intravenous catheter can be slid over the barbell threads to maintain the piercing tract during the scan.

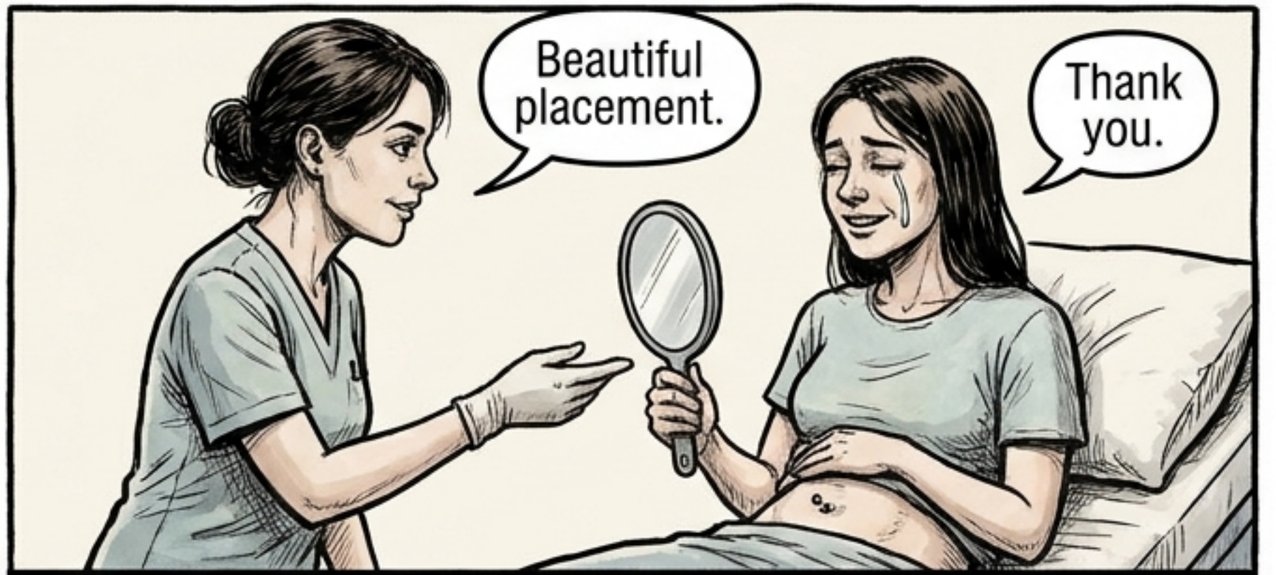

They had successfully converted a highly advanced medical suite into a temporary body modification studio.