


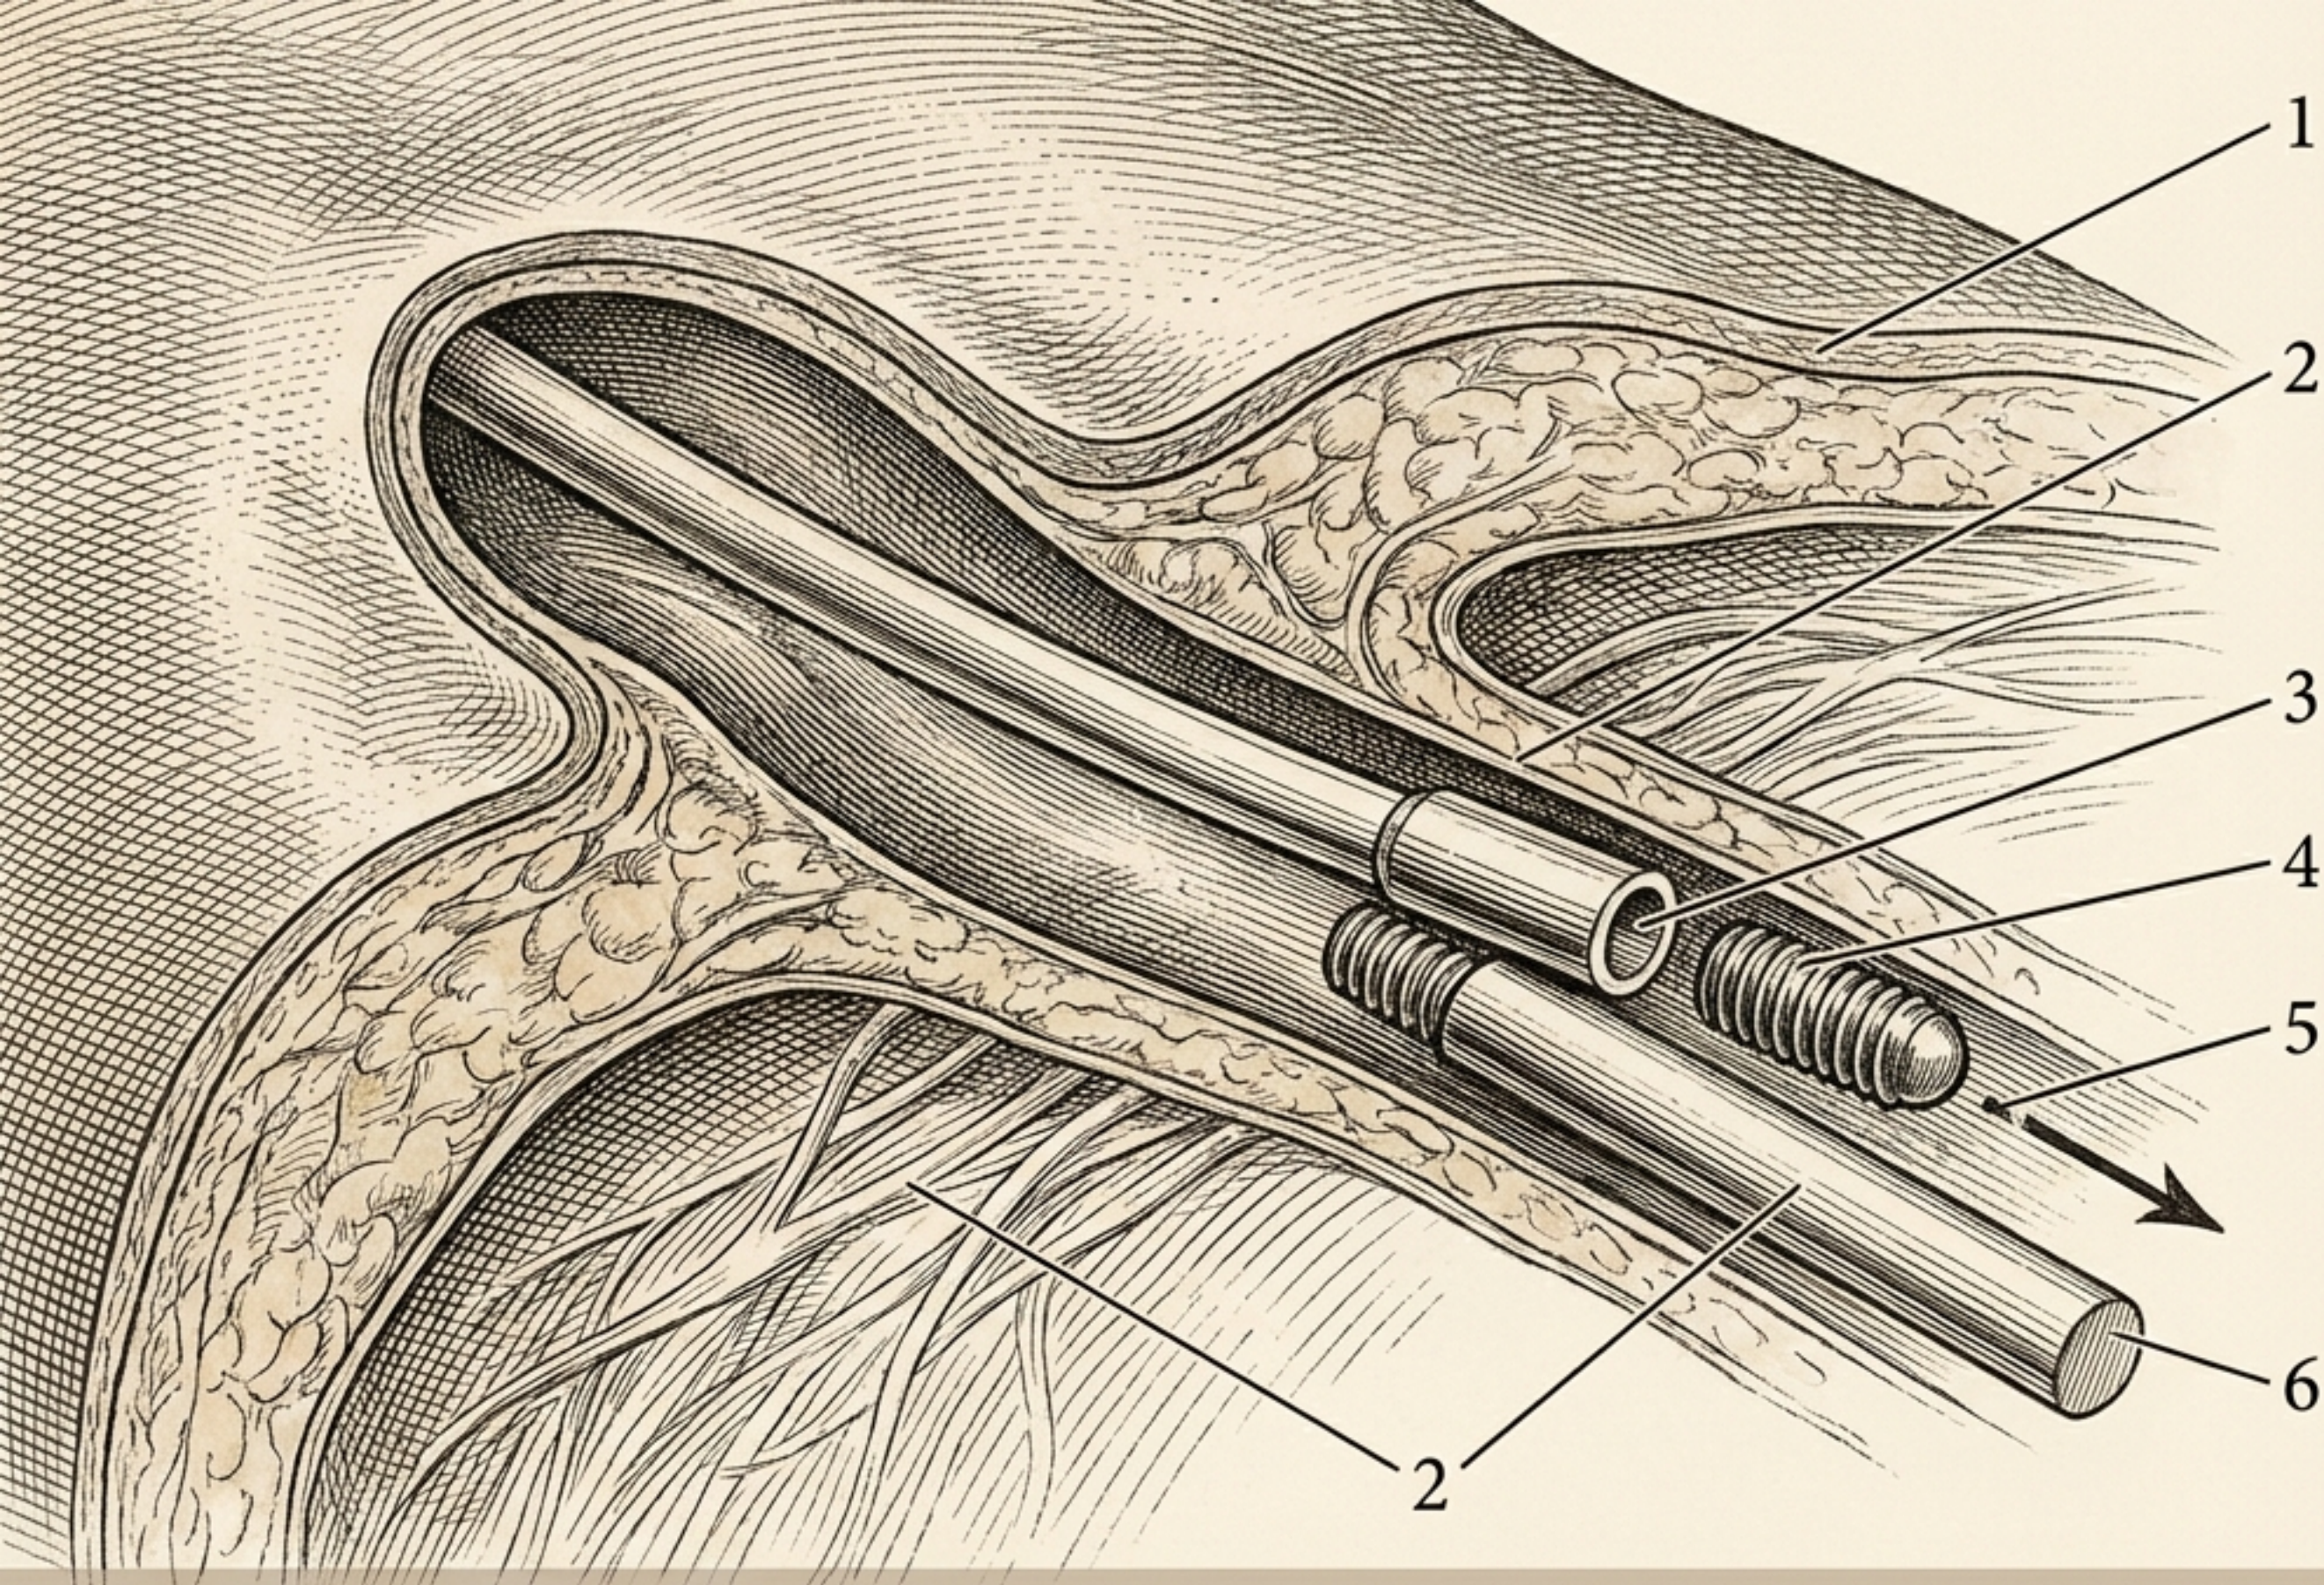

- 1. Umbilical area epidermis
- 2. Subcutaneous skin tract
- 3. Threaded bar tip
- 4. 14 gauge intravenous catheter
- 5. Pushing piercing out caudally
- 6. Nonmetallic spacer remains

A tight-fitting intravenous catheter serves as a nonmetallic spacer during imaging.
PRESERVE TRACTS WITH NONMETALLIC RETAINERS.