


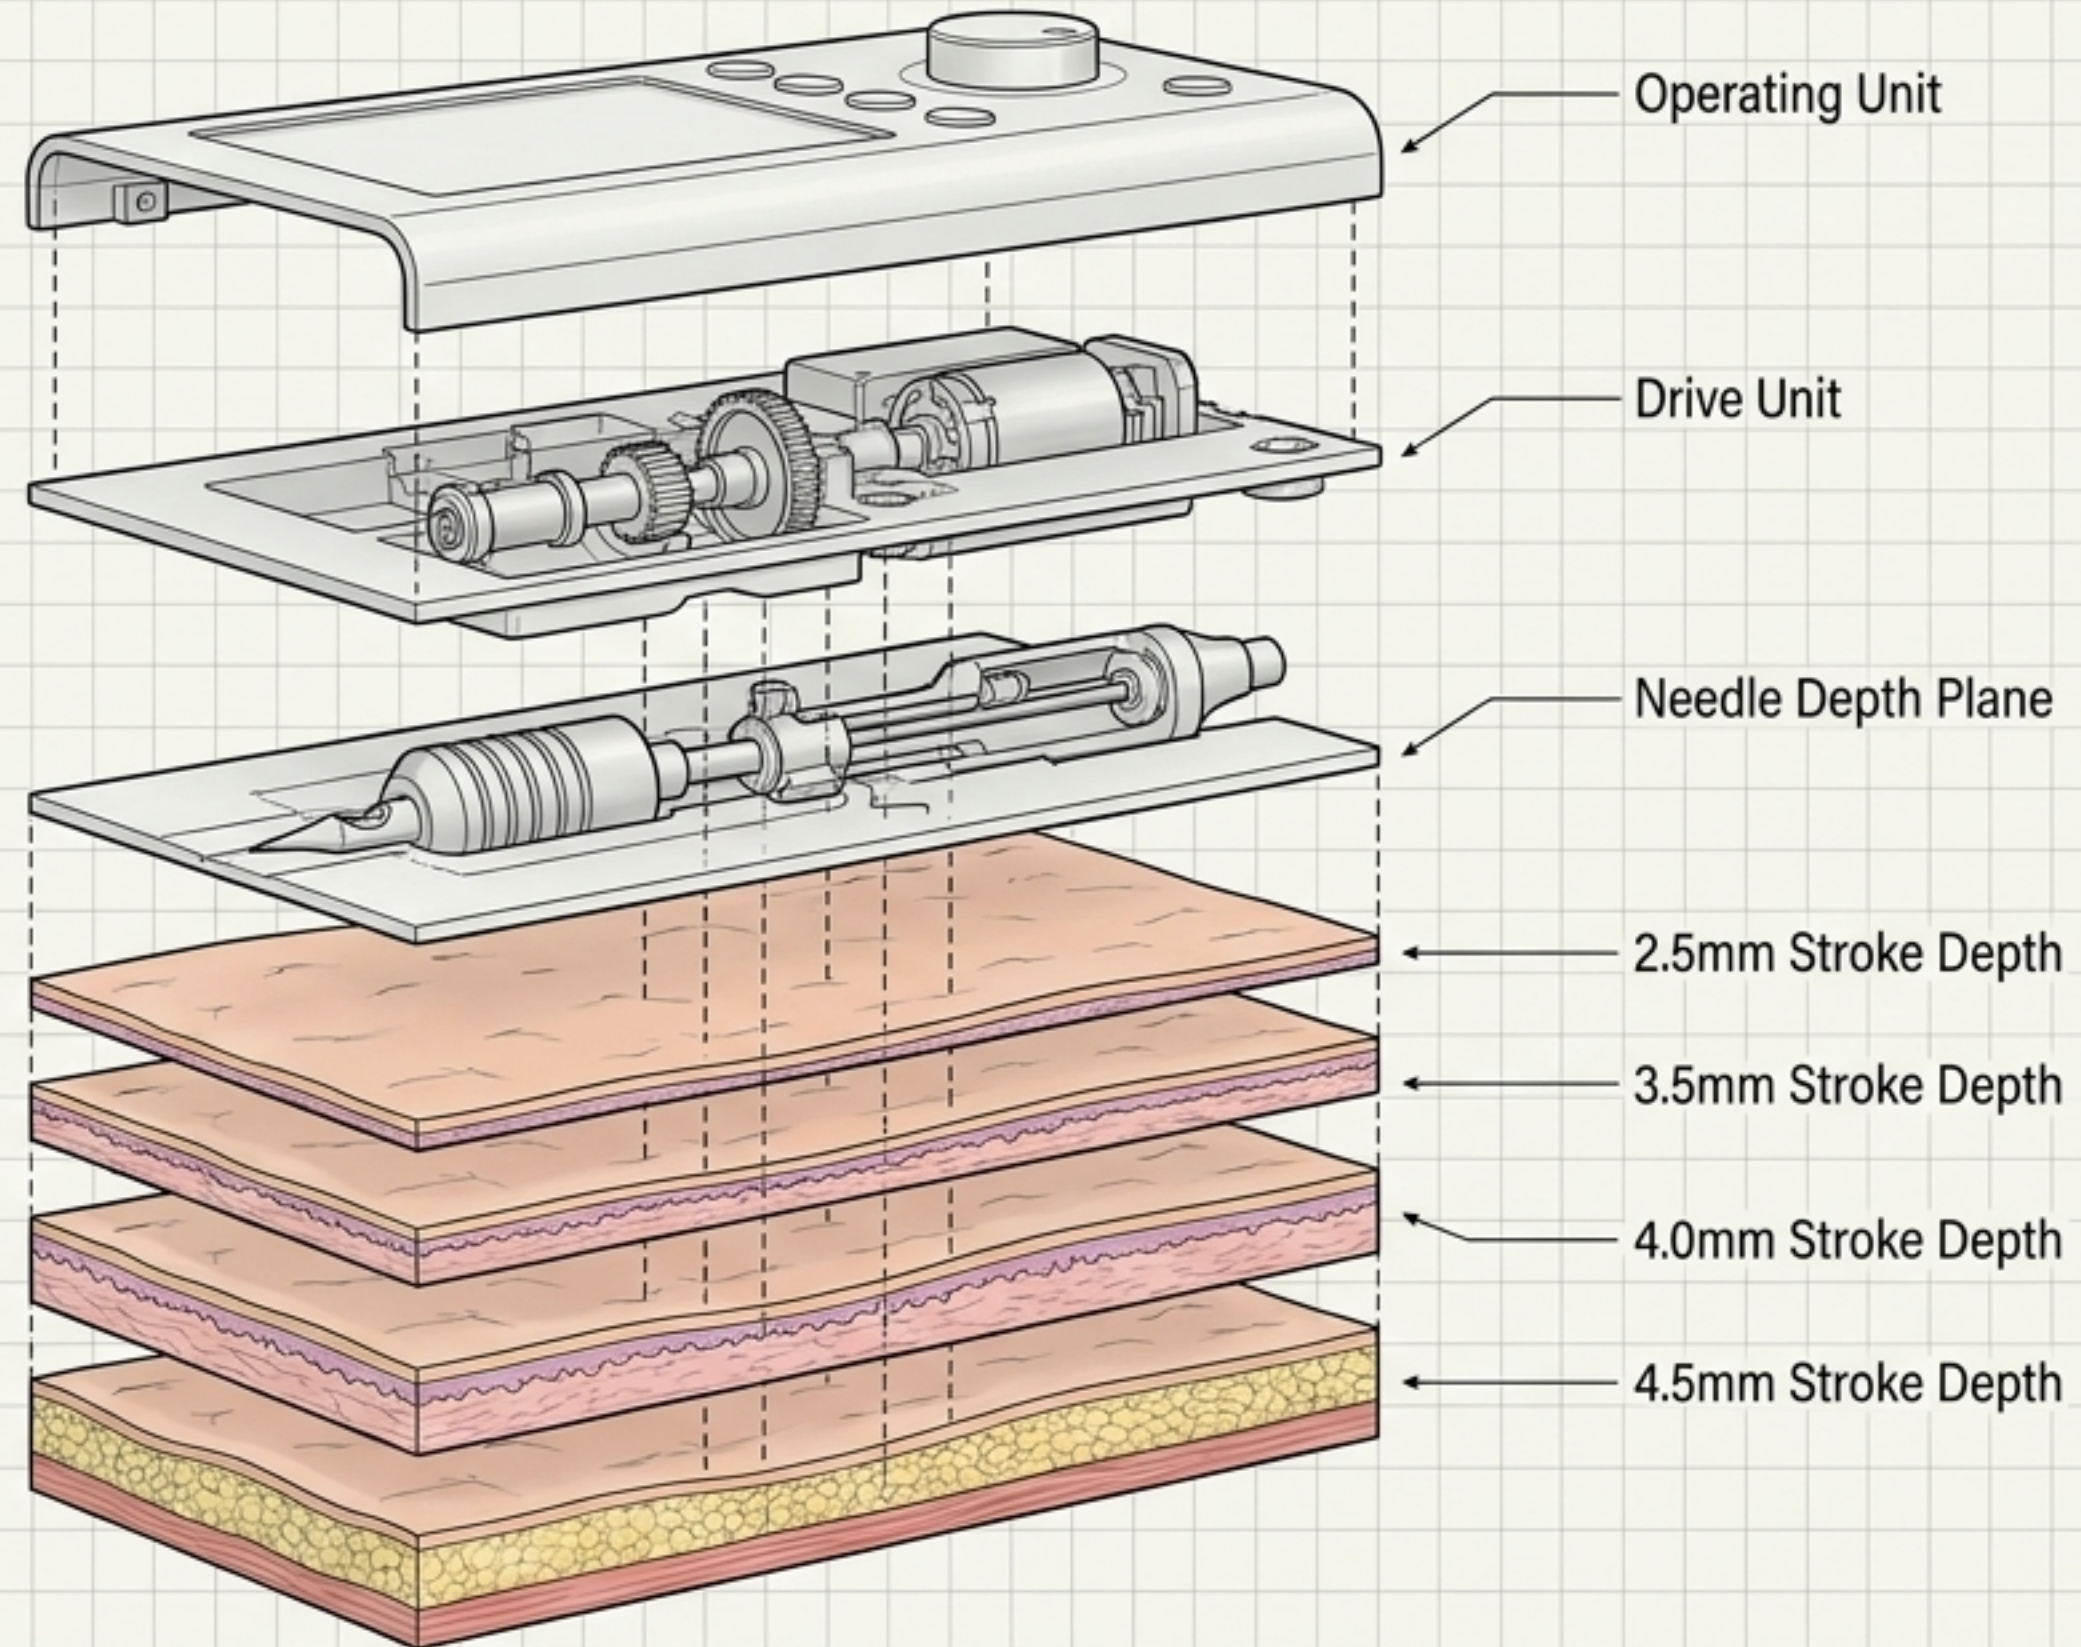

The modular drive unit separates from the power supply to deliver four precise stroke depths into the tissue.

MODULAR DEPTH AND POWER