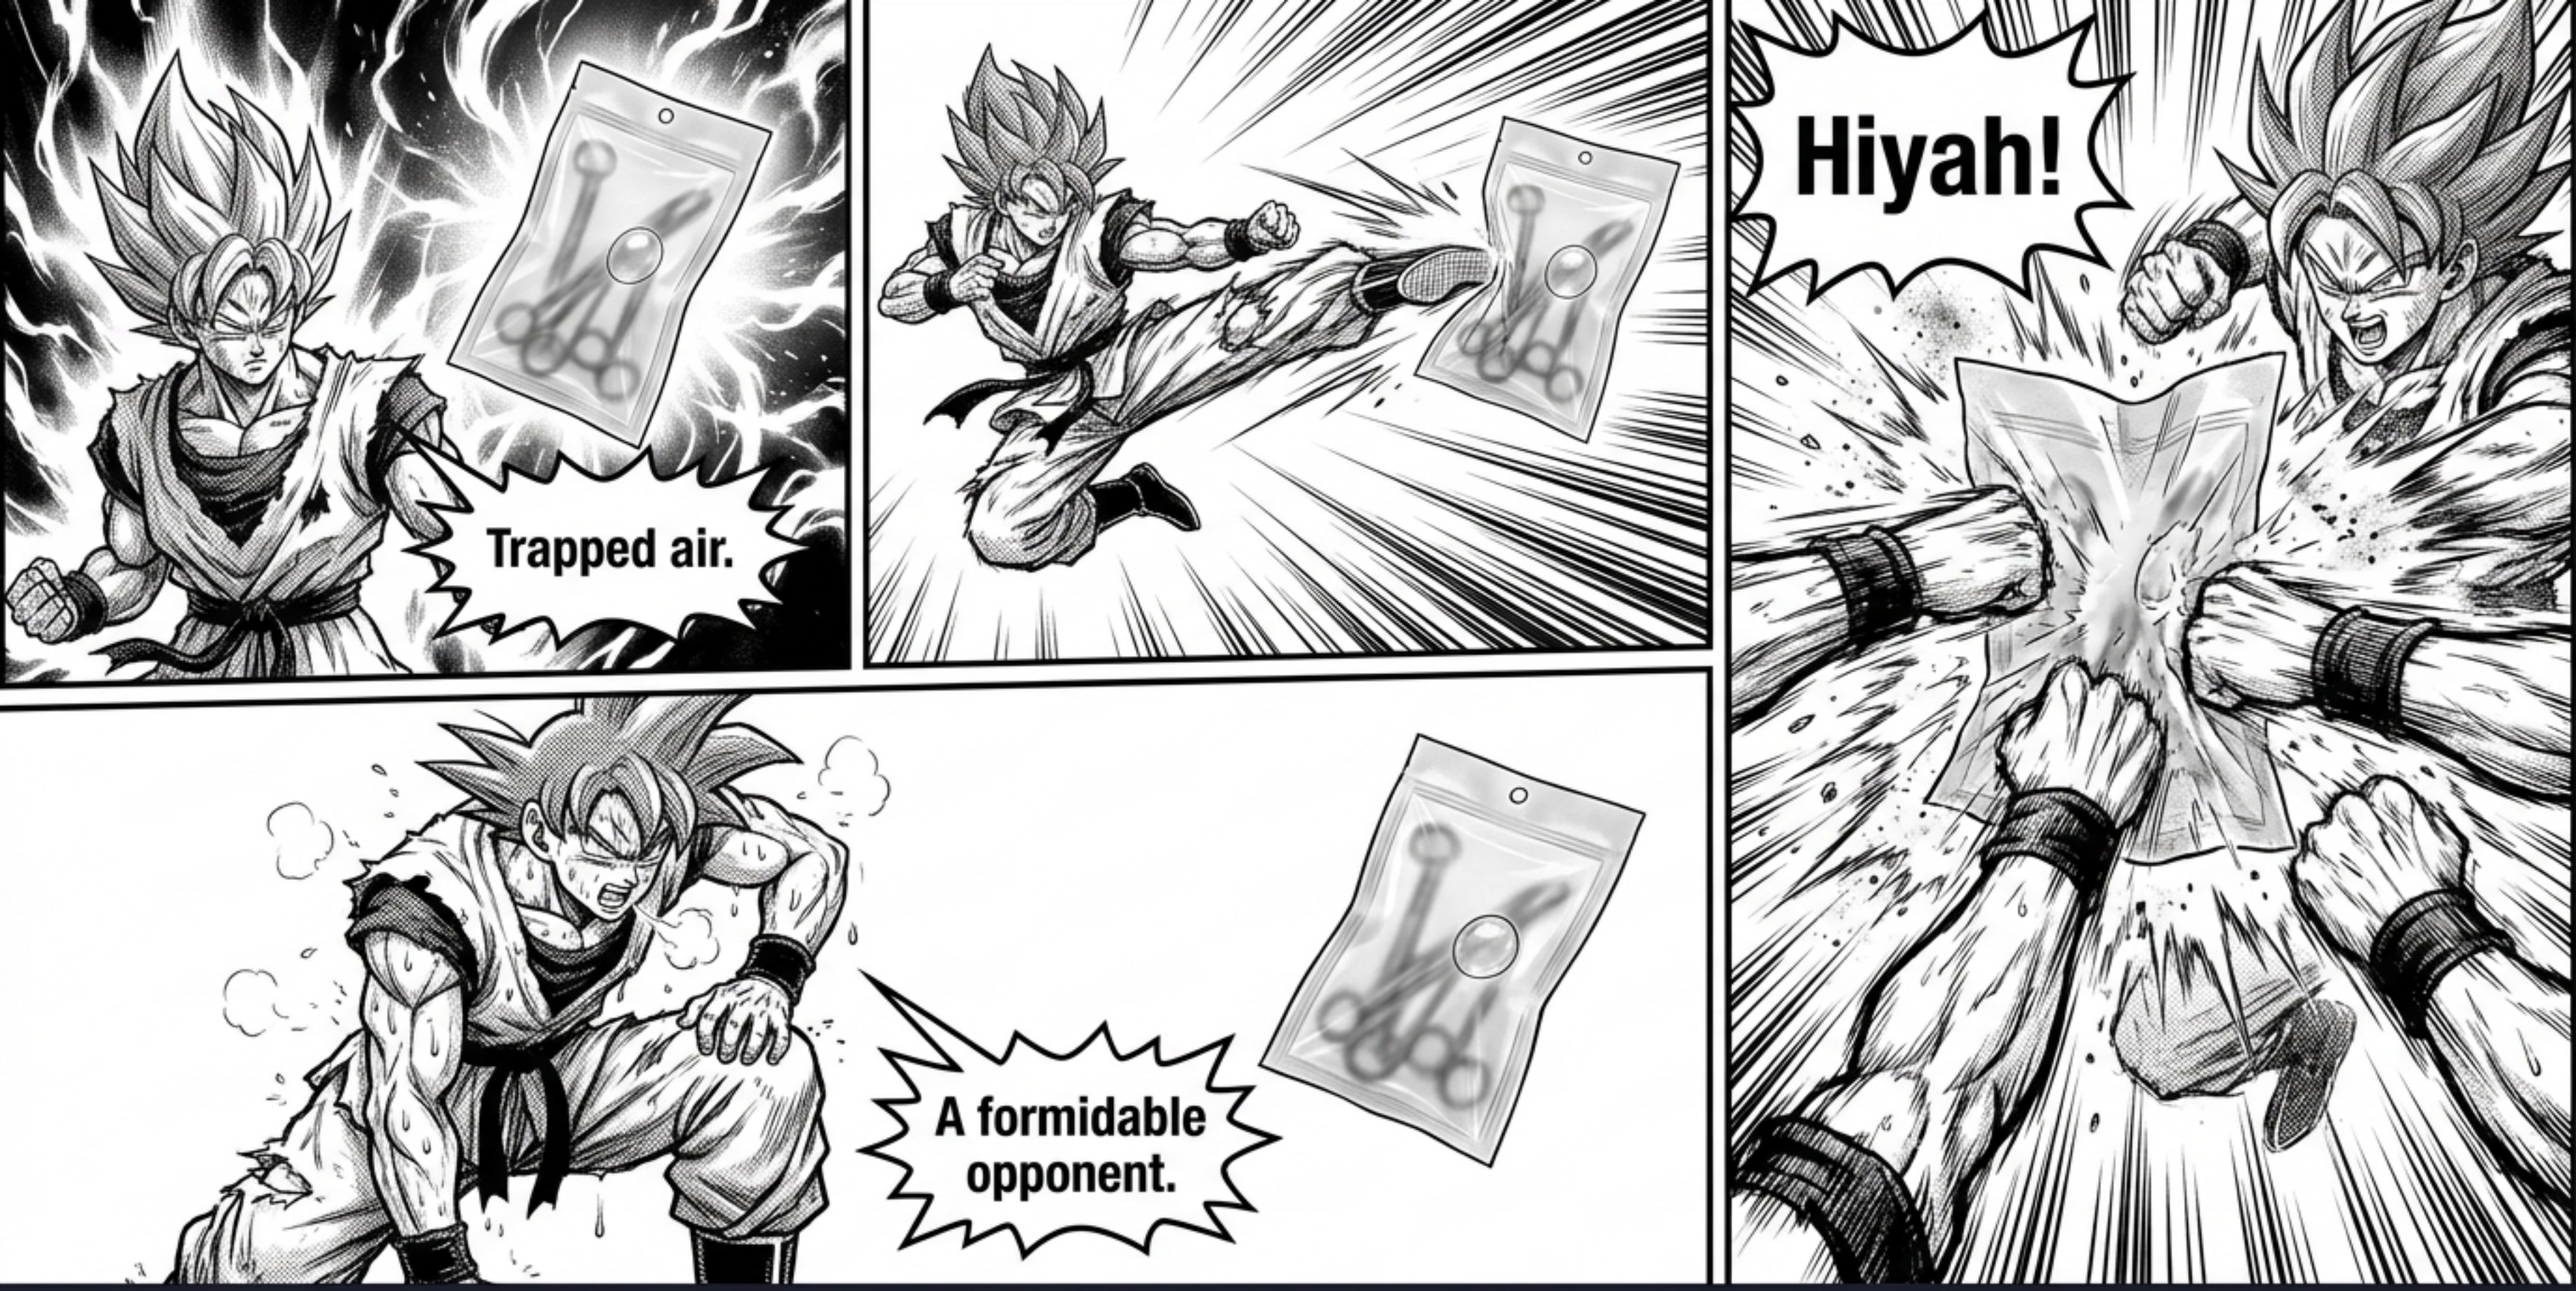

Gravity displacement autoclaves lack the active vacuum phase required to extract trapped air pockets from inside wrapped instruments.

Invisible atmospheric shields require a completely different combat strategy.