


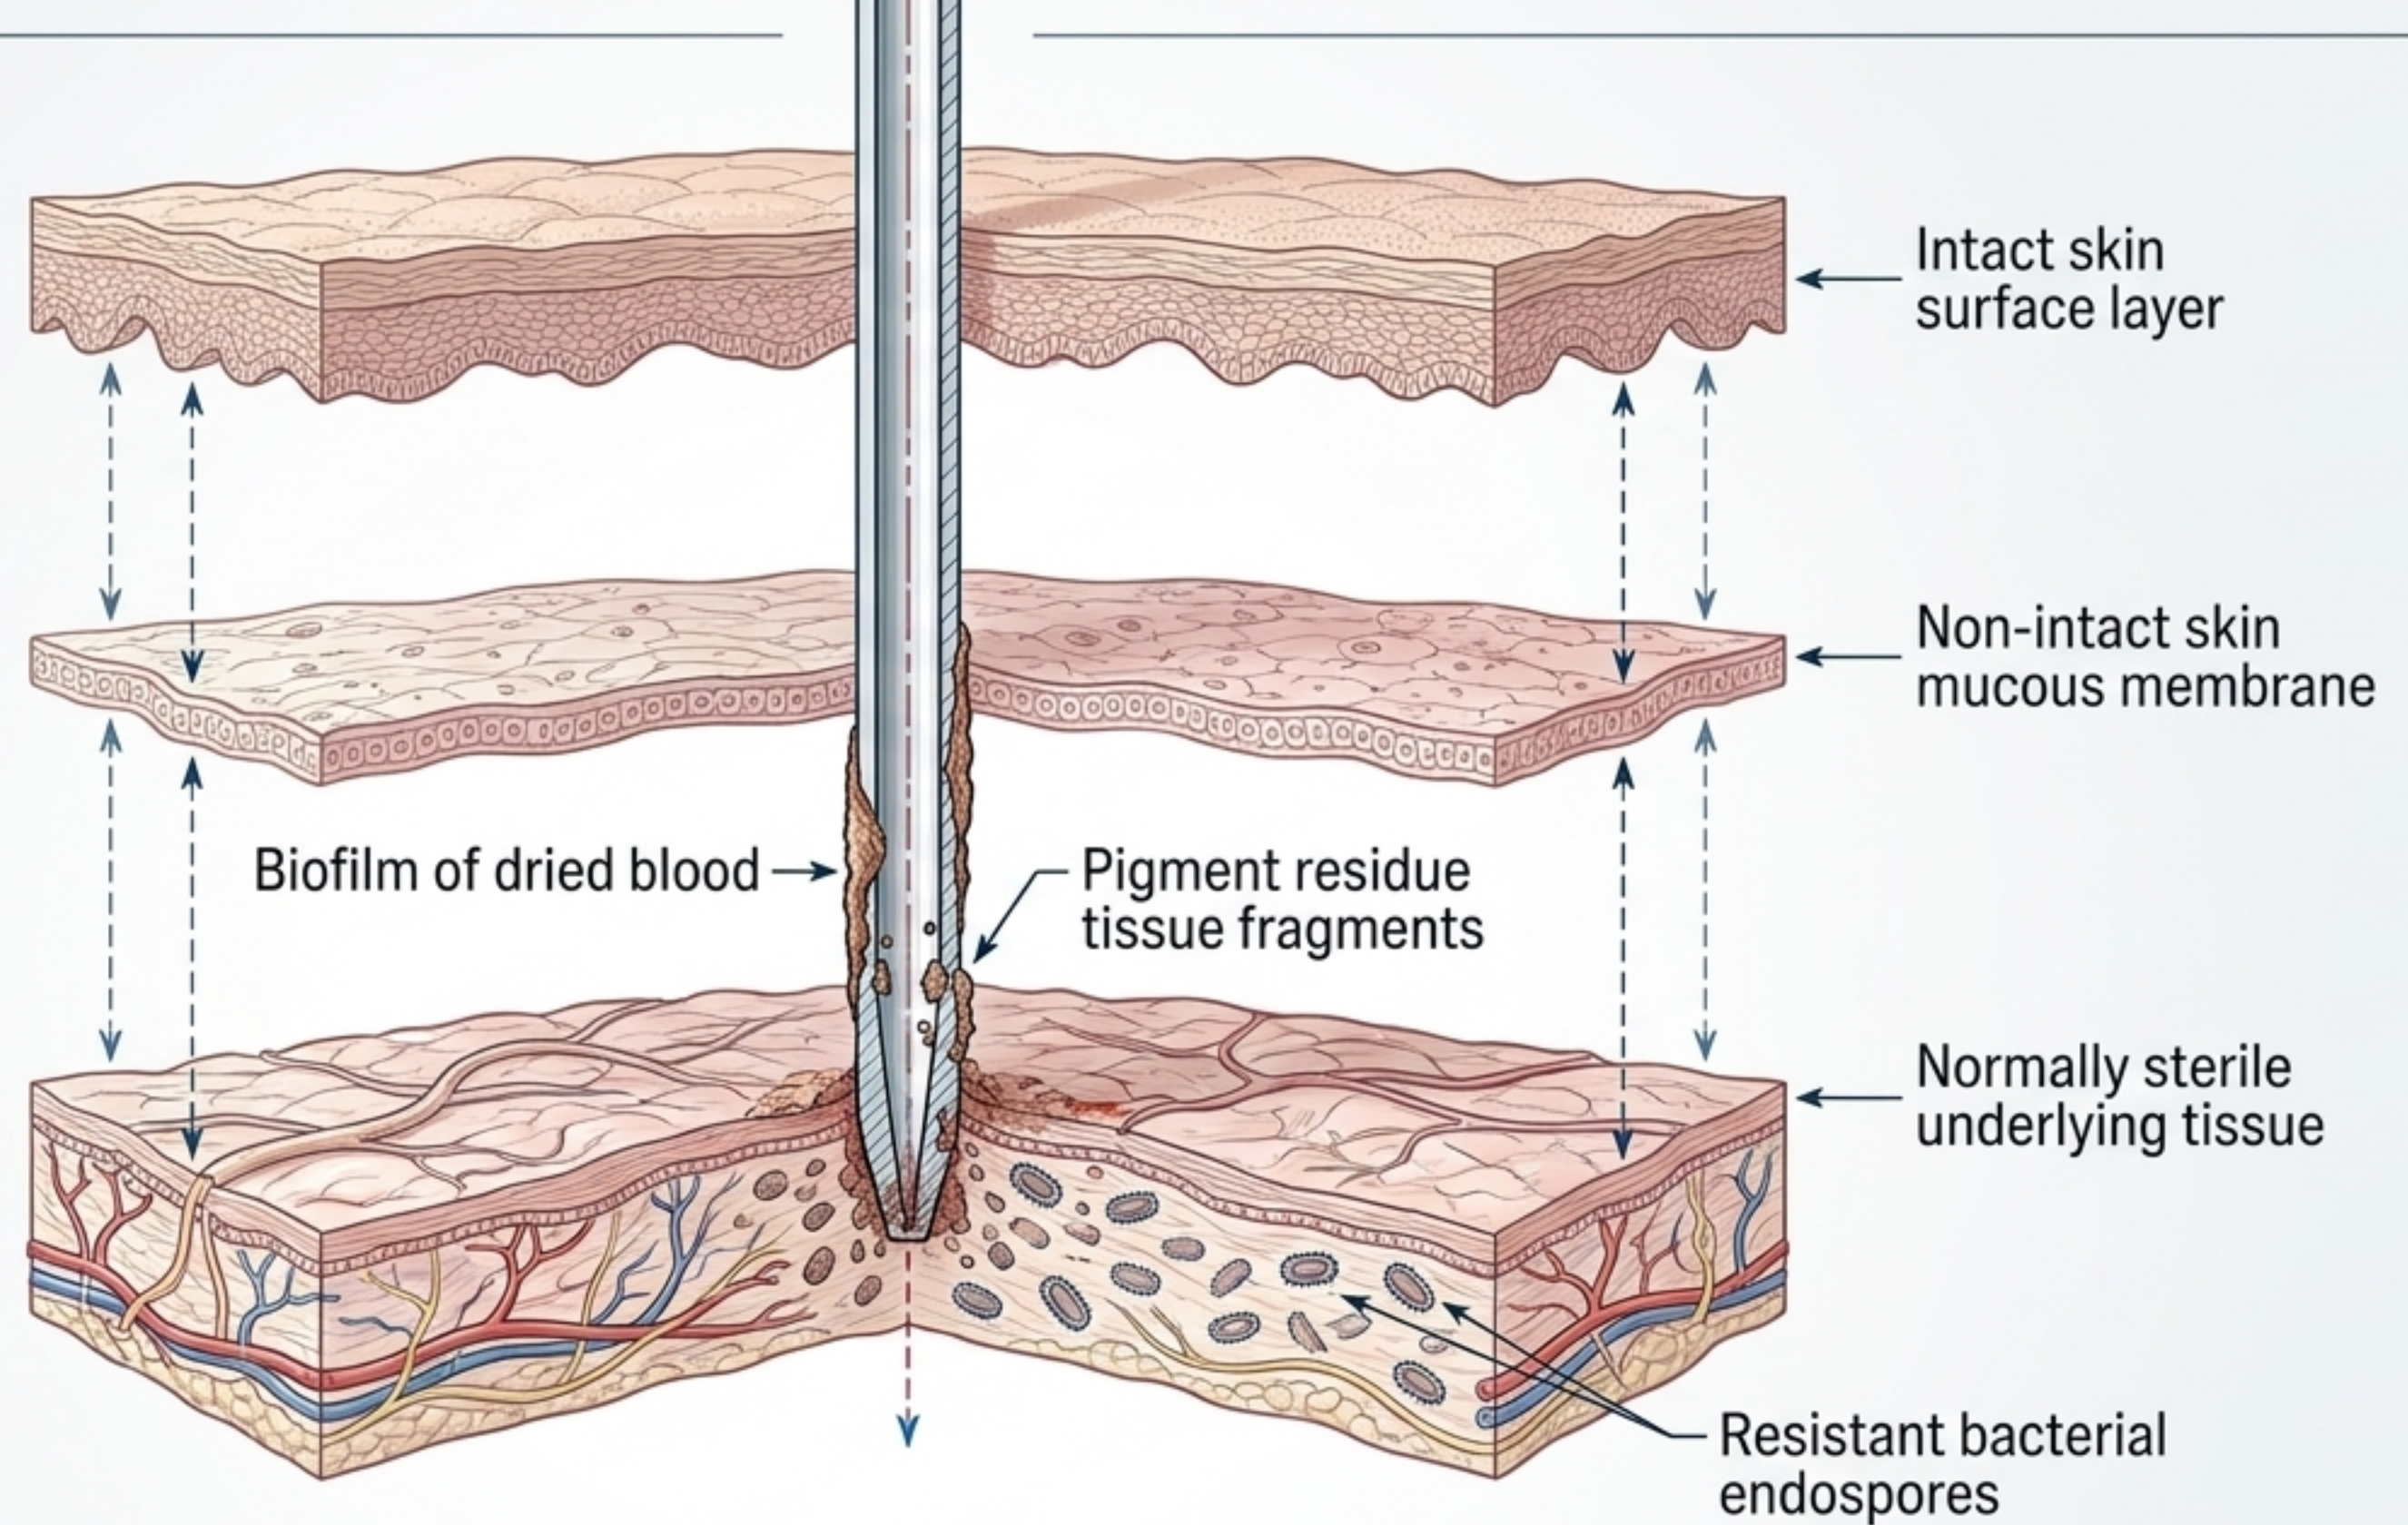

Instruments penetrating into sterile tissue or blood must be entirely free of shielding biofilms and endospores.

STERILIZATION DESTROYS ALL MICROBIAL LIFE