


DO NOT use spring loaded piercing guns.



Blunt force trauma crushes the perichondrium.

Crushed tissue separates from the cartilage.

DO use sharp surgical piercing needles.

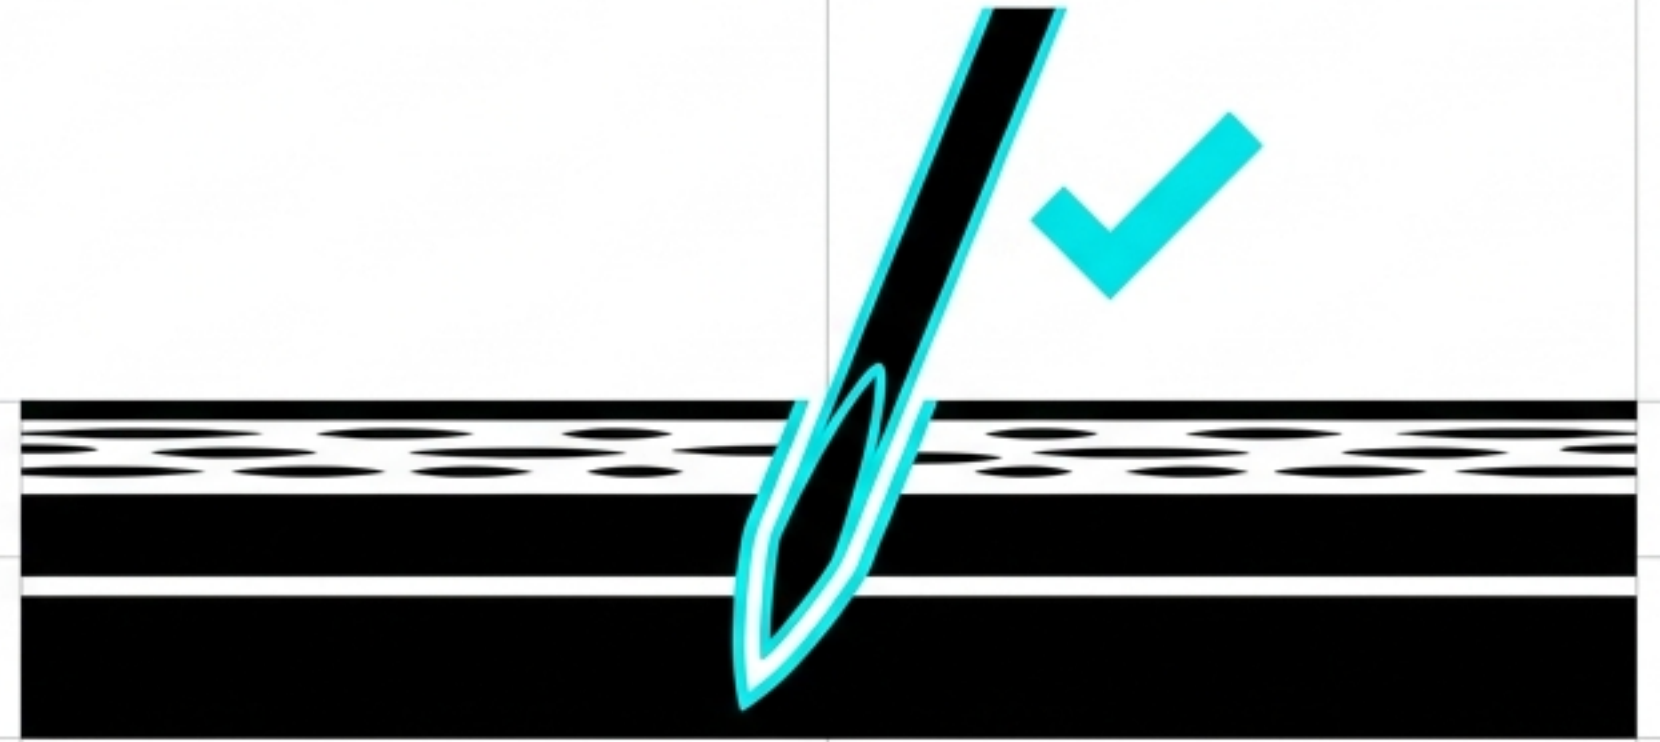

Needles create clean smooth tissue separation.

Clean separation preserves the cellular structure.

Plastic ear piercing guns cannot be steam autoclave sterilized. ONLY USE STERILE DISPOSABLE EQUIPMENT.