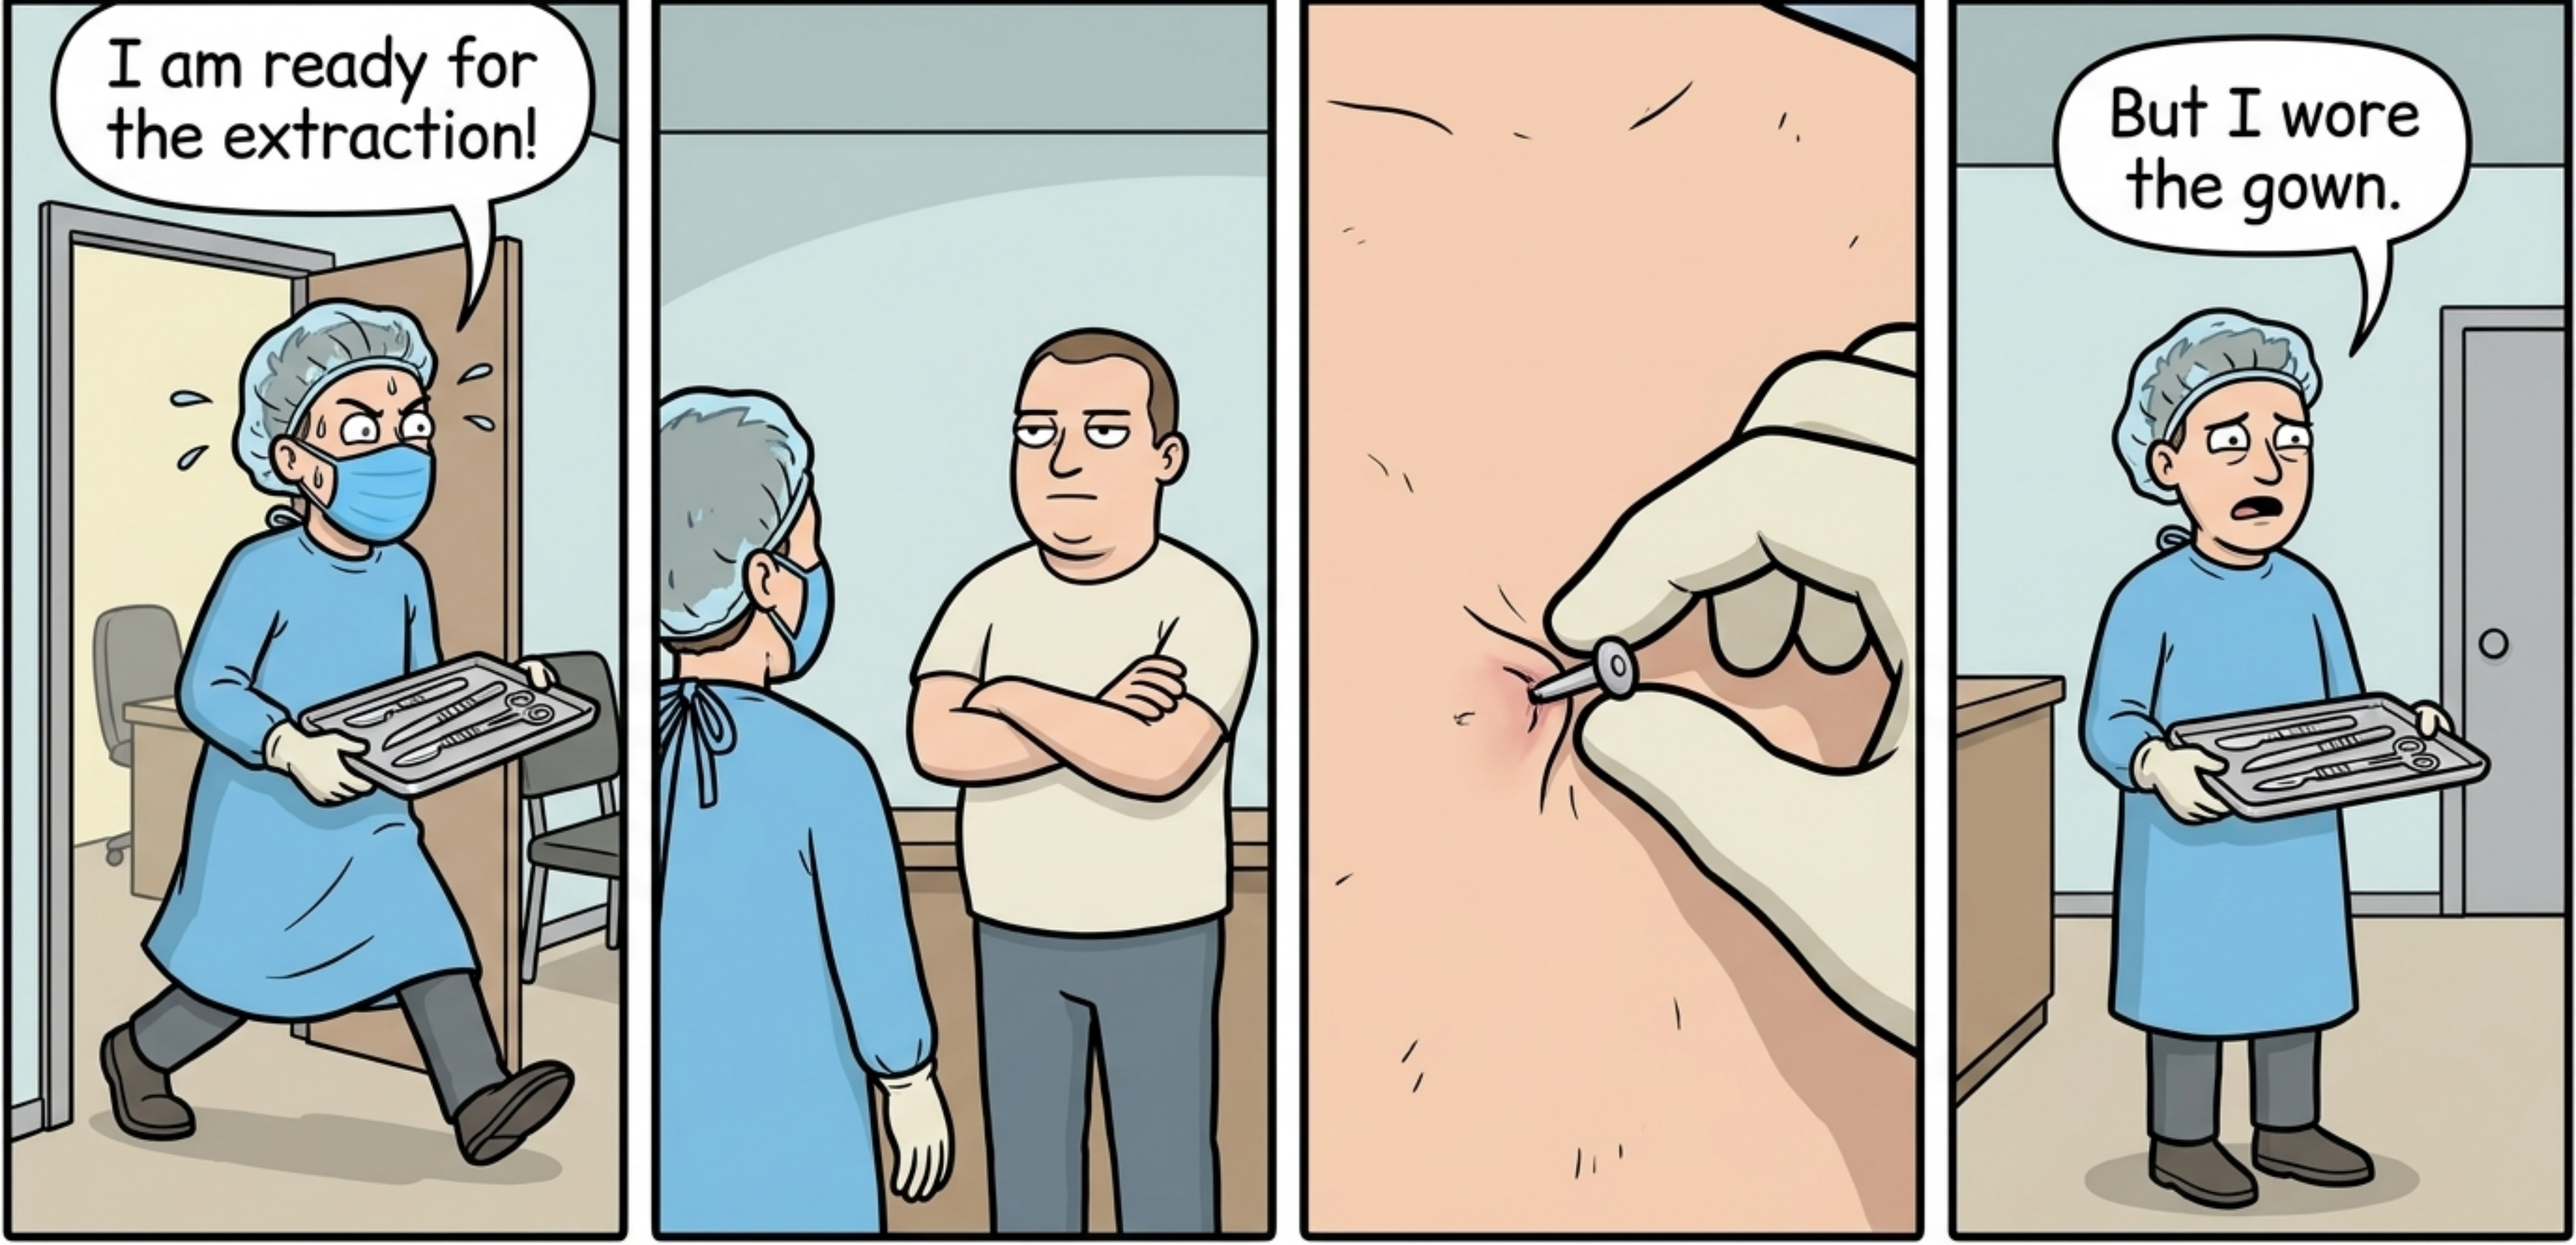

Surface anchors do not require surgical excision and can be removed by tissue manipulation.
Canceling the operating theatre leaves more time for lunch.