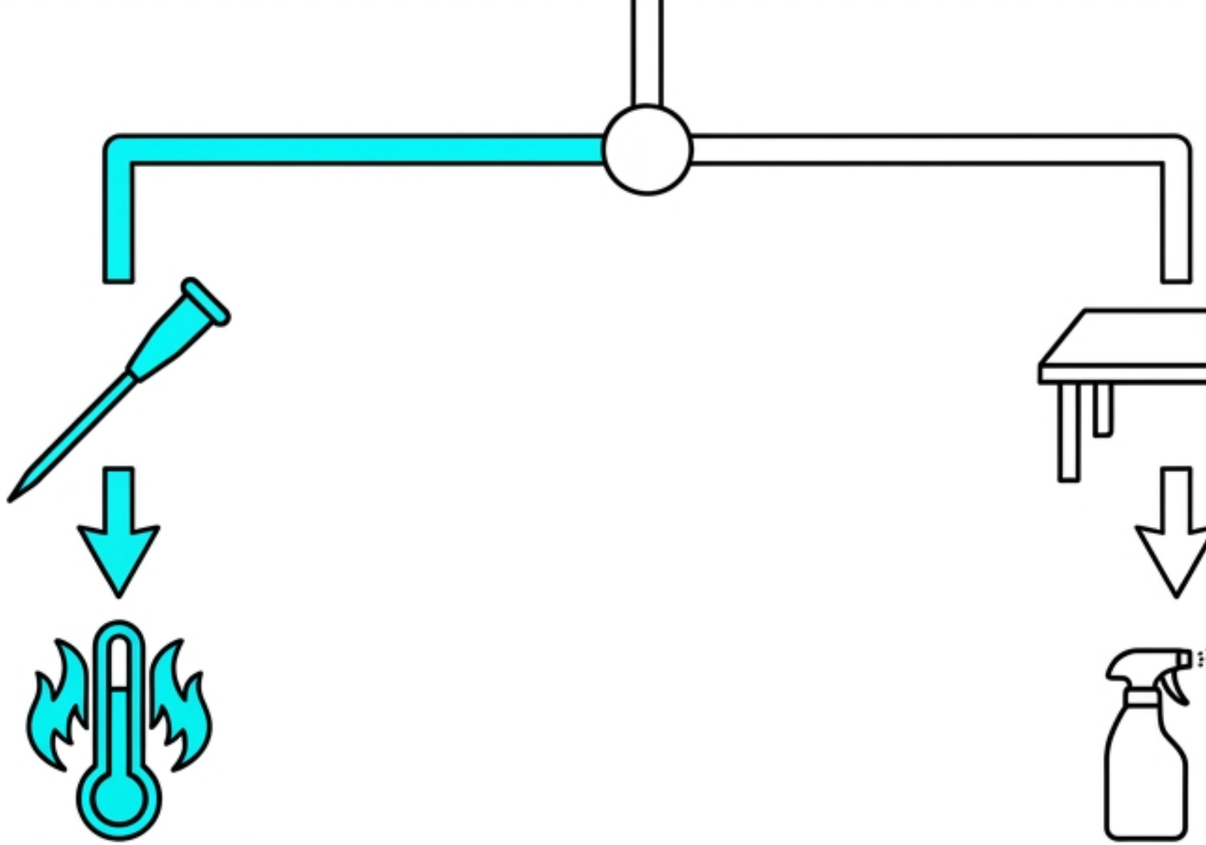

Sterilization destroys all microbial life forms.

Autoclave all skin penetrating tools.

Disinfection reduces germs to safe levels.

Disinfect non porous environmental surfaces only.

Autoclaves must reach 121 to 134 degrees Celsius.

NEVER USE DISINFECTANT ON PIERCING TOOLS.