


BODY JEWELRY MUST FEATURE INTERNAL TAPPING.
IMPLANT TITANIUM COMPLIES WITH ASTM F136.
IMPLANT STEEL COMPLIES WITH ASTM F138.
SOLID GOLD REQUIRES MINIMUM 14 KARATS.

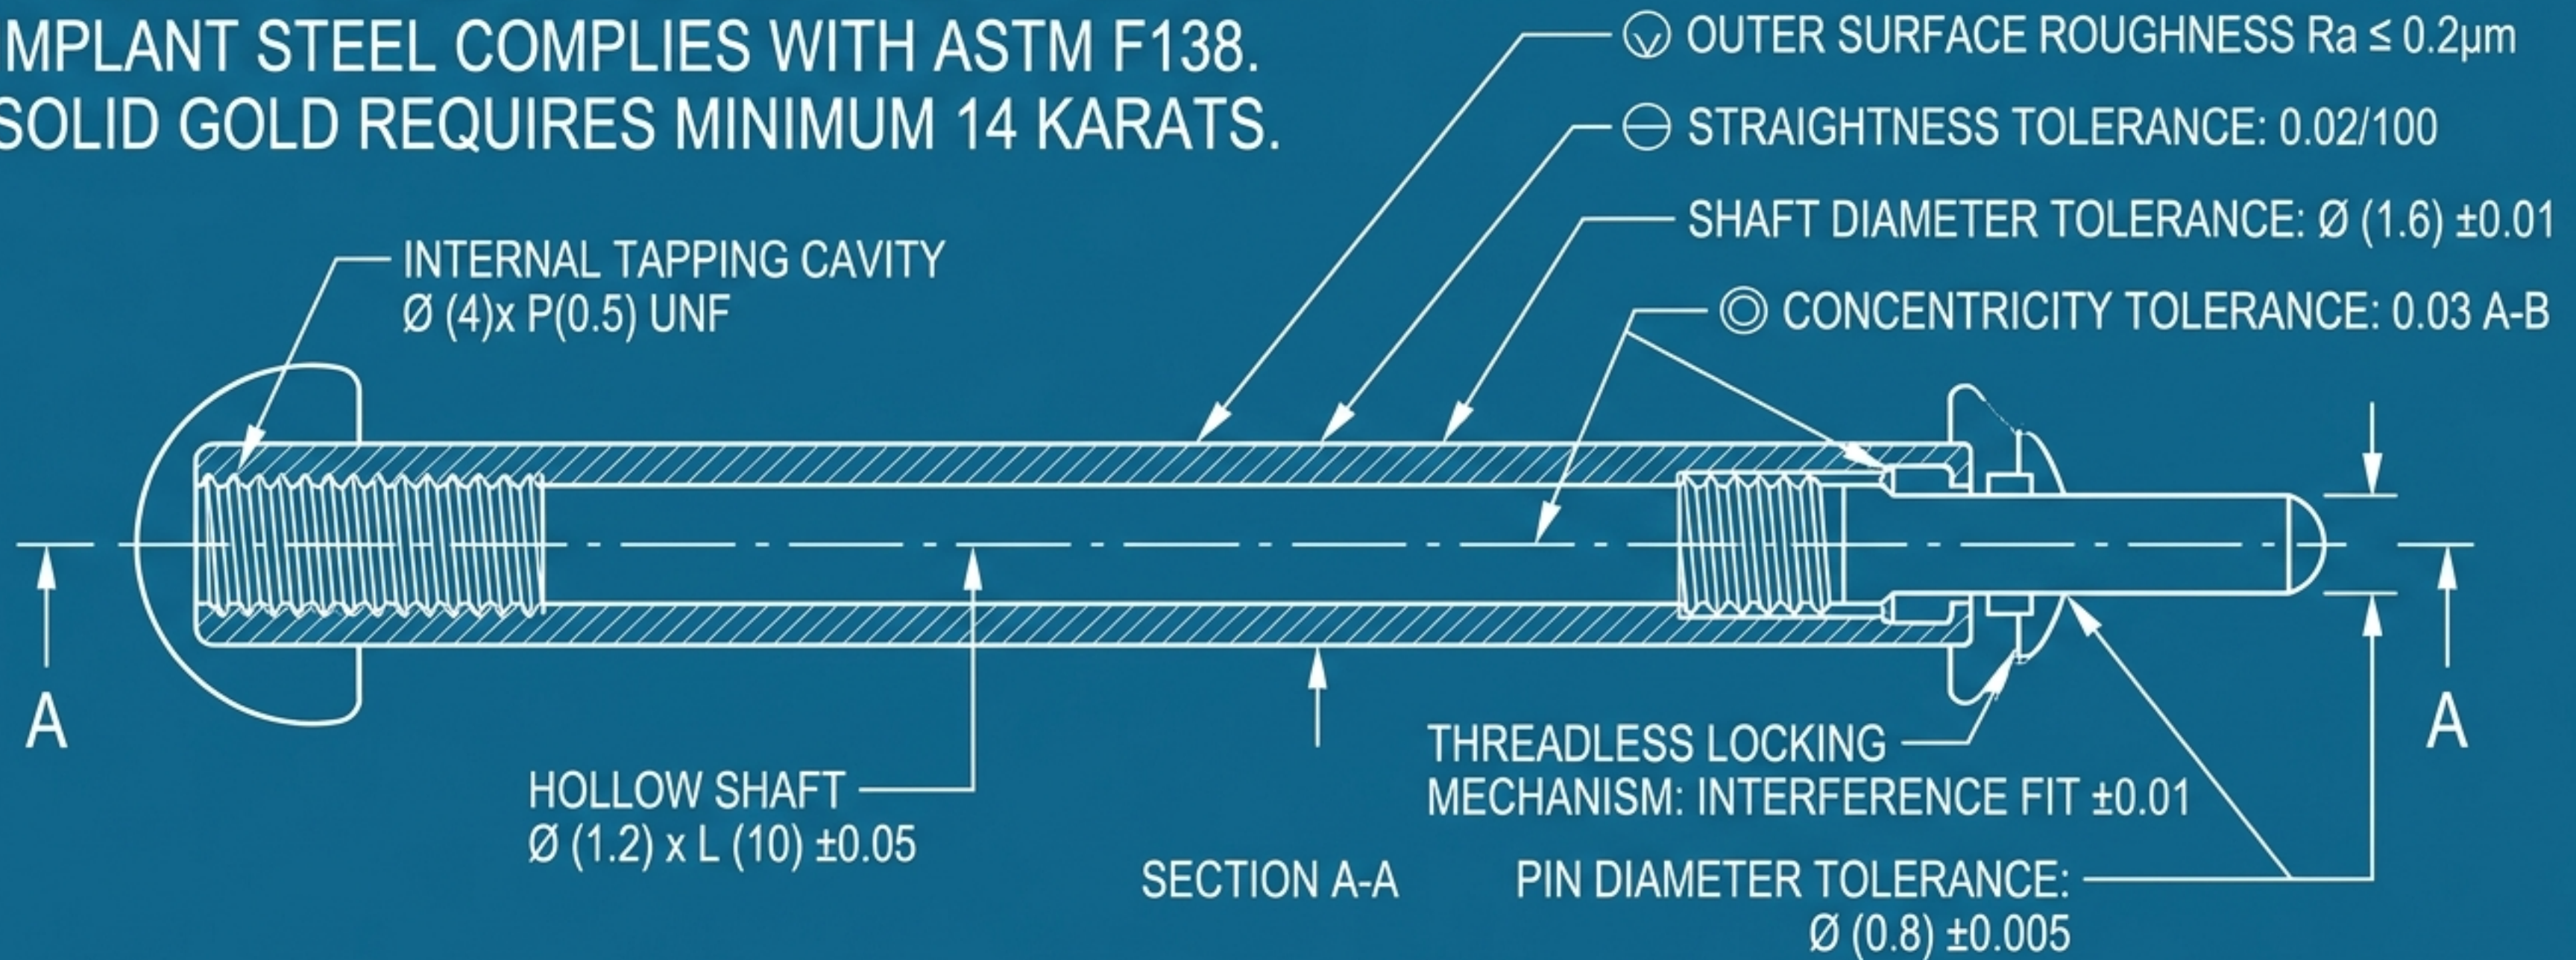

Internal threading prevents tissue tearing during insertion.
NO EXTERIOR THREADS ALLOWED.