Steam sterilization degrades flexible polymers.
Copolymers withstand limited thermal cycles.
Degradation begins after maximum cycles.
Heat reaches 134 degrees inside.
Limit exposure to 8 cycles.
Discard items after 12 cycles.

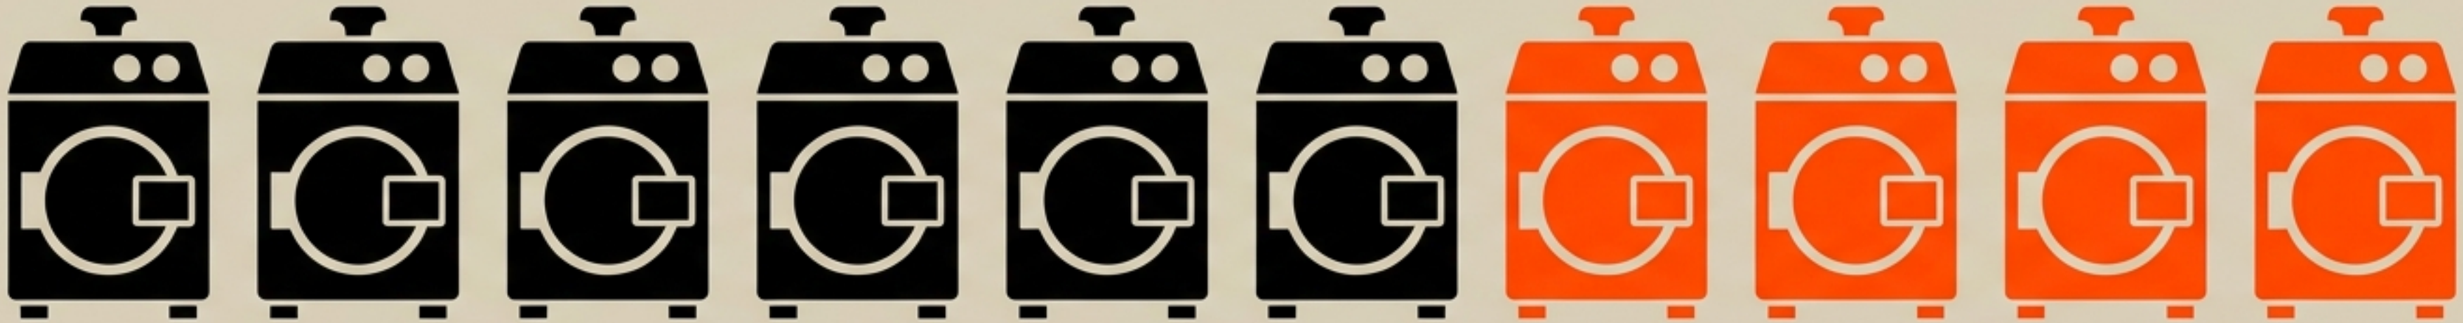

Medical copolymers survive a limited number of extreme steam sterilization cycles.
TRACK YOUR CYCLES

Gemini Notebook