


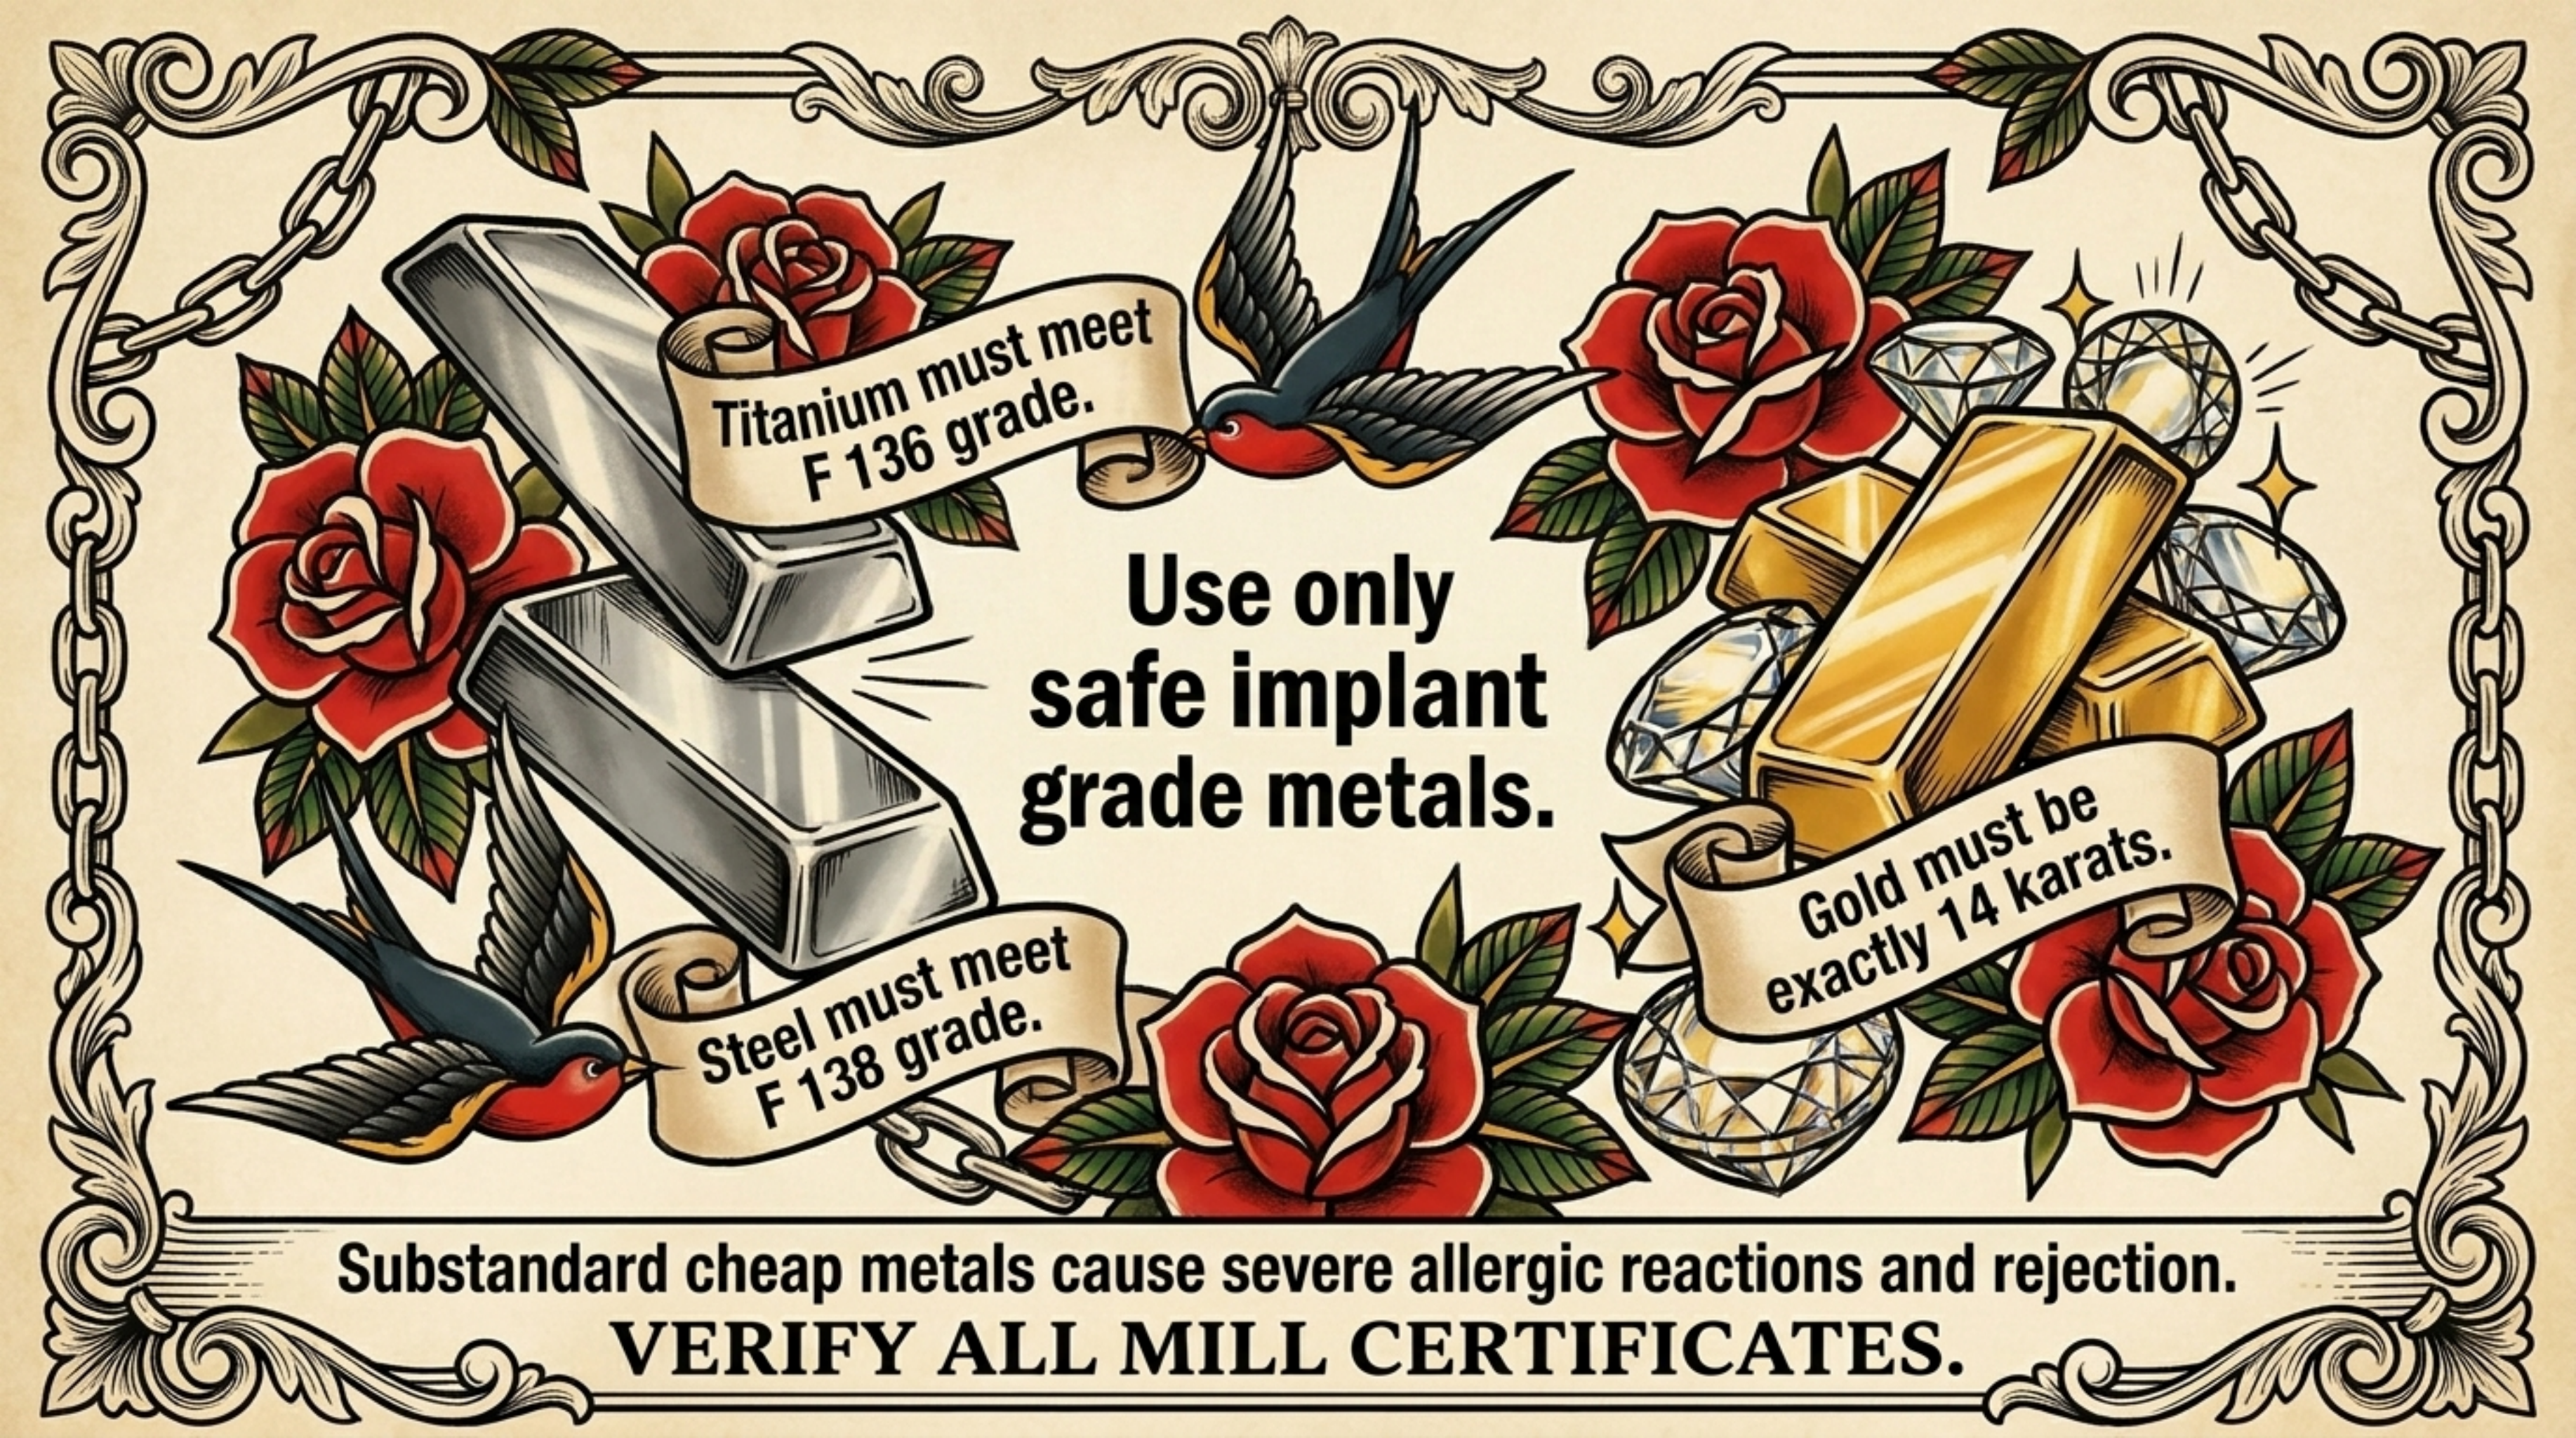

Titanium must meet
F 136 grade.

**Use only
safe implant
grade metals.**

Steel must meet
F 138 grade.

Gold must be
exactly 14 karats.

Substandard cheap metals cause severe allergic reactions and rejection.
VERIFY ALL MILL CERTIFICATES.