


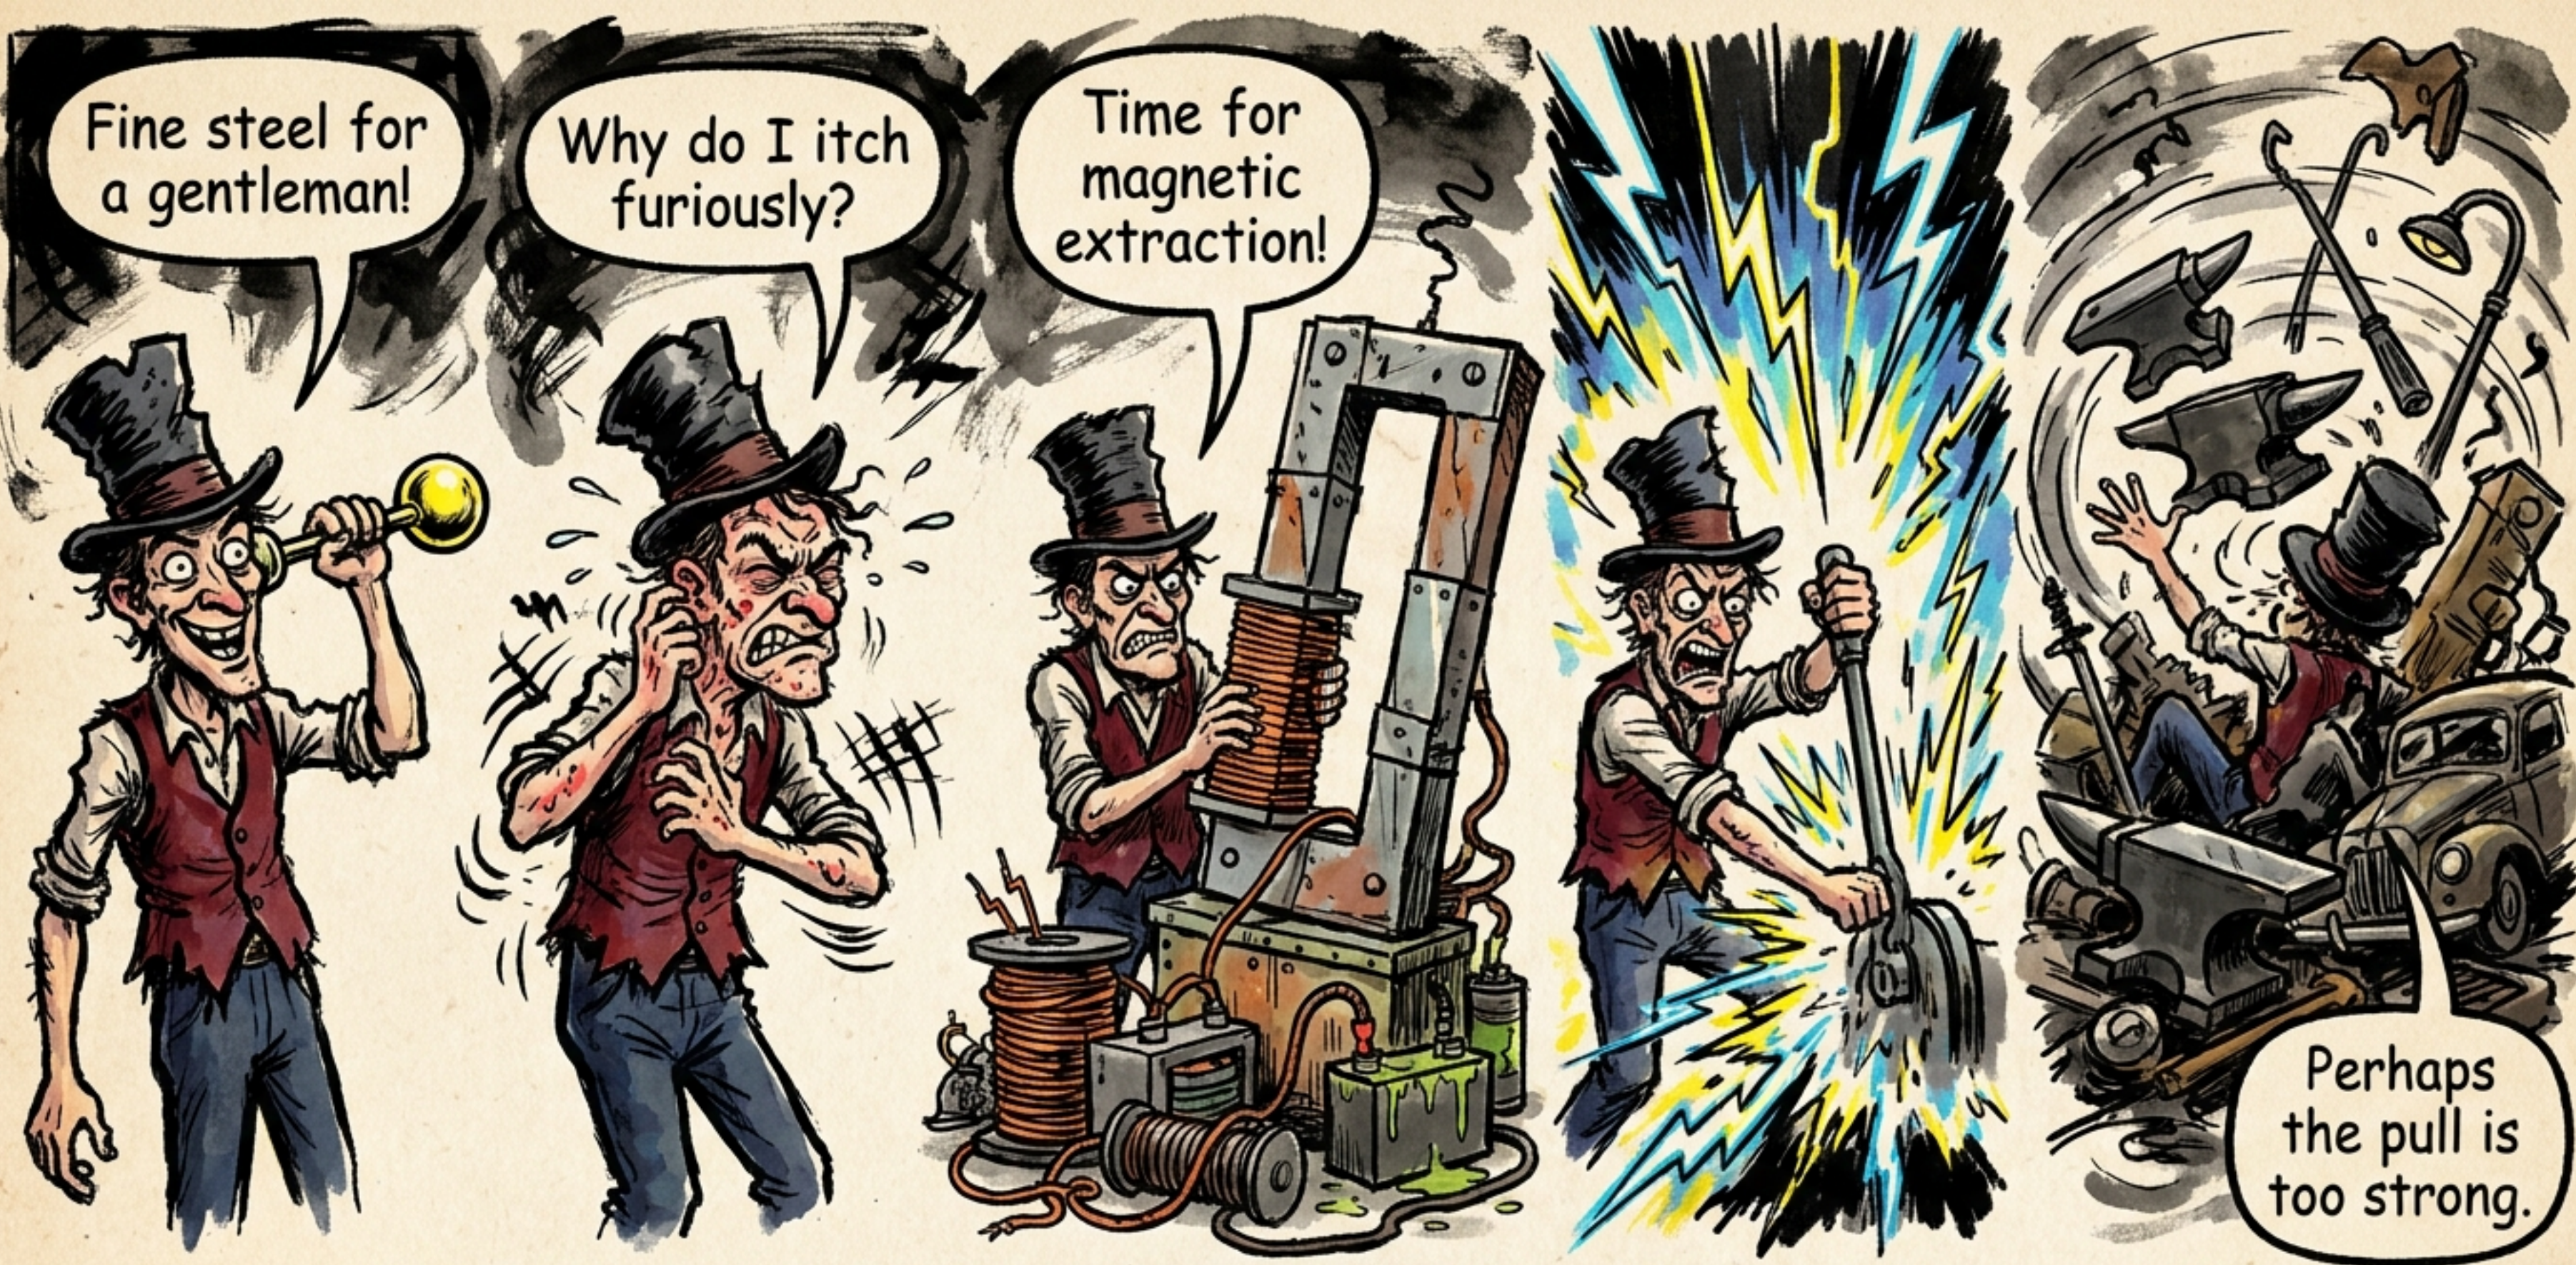

Surgical steel contains nickel which leaches into contacted tissue and causes allergic reactions. The bespoke extraction magnet requires its own dedicated power grid.