
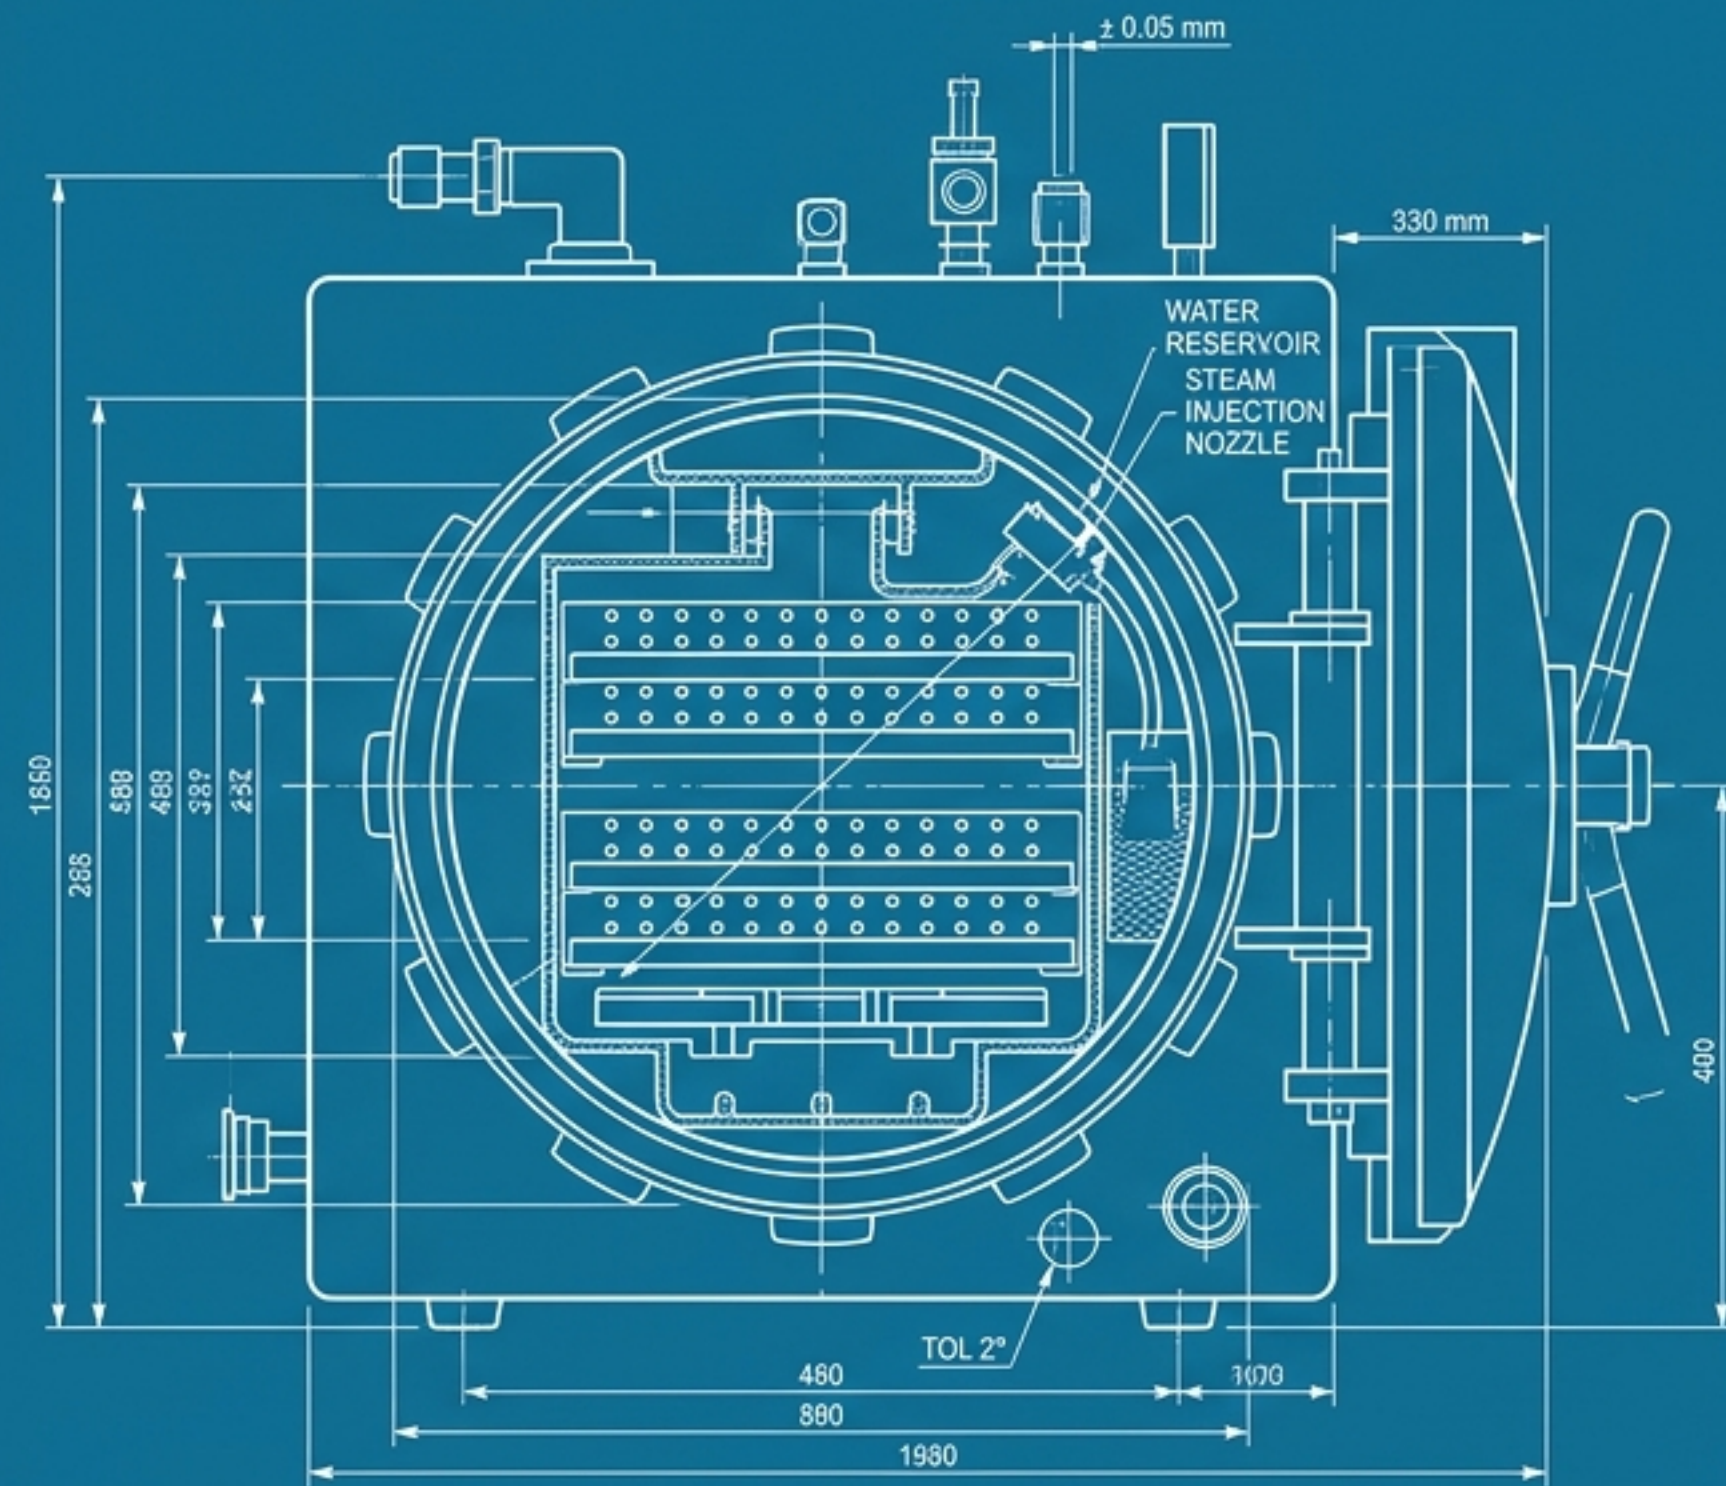


B-Cycle steam sterilization requirements
Target pressure is 2.1 bar
Hold duration is 5 minutes

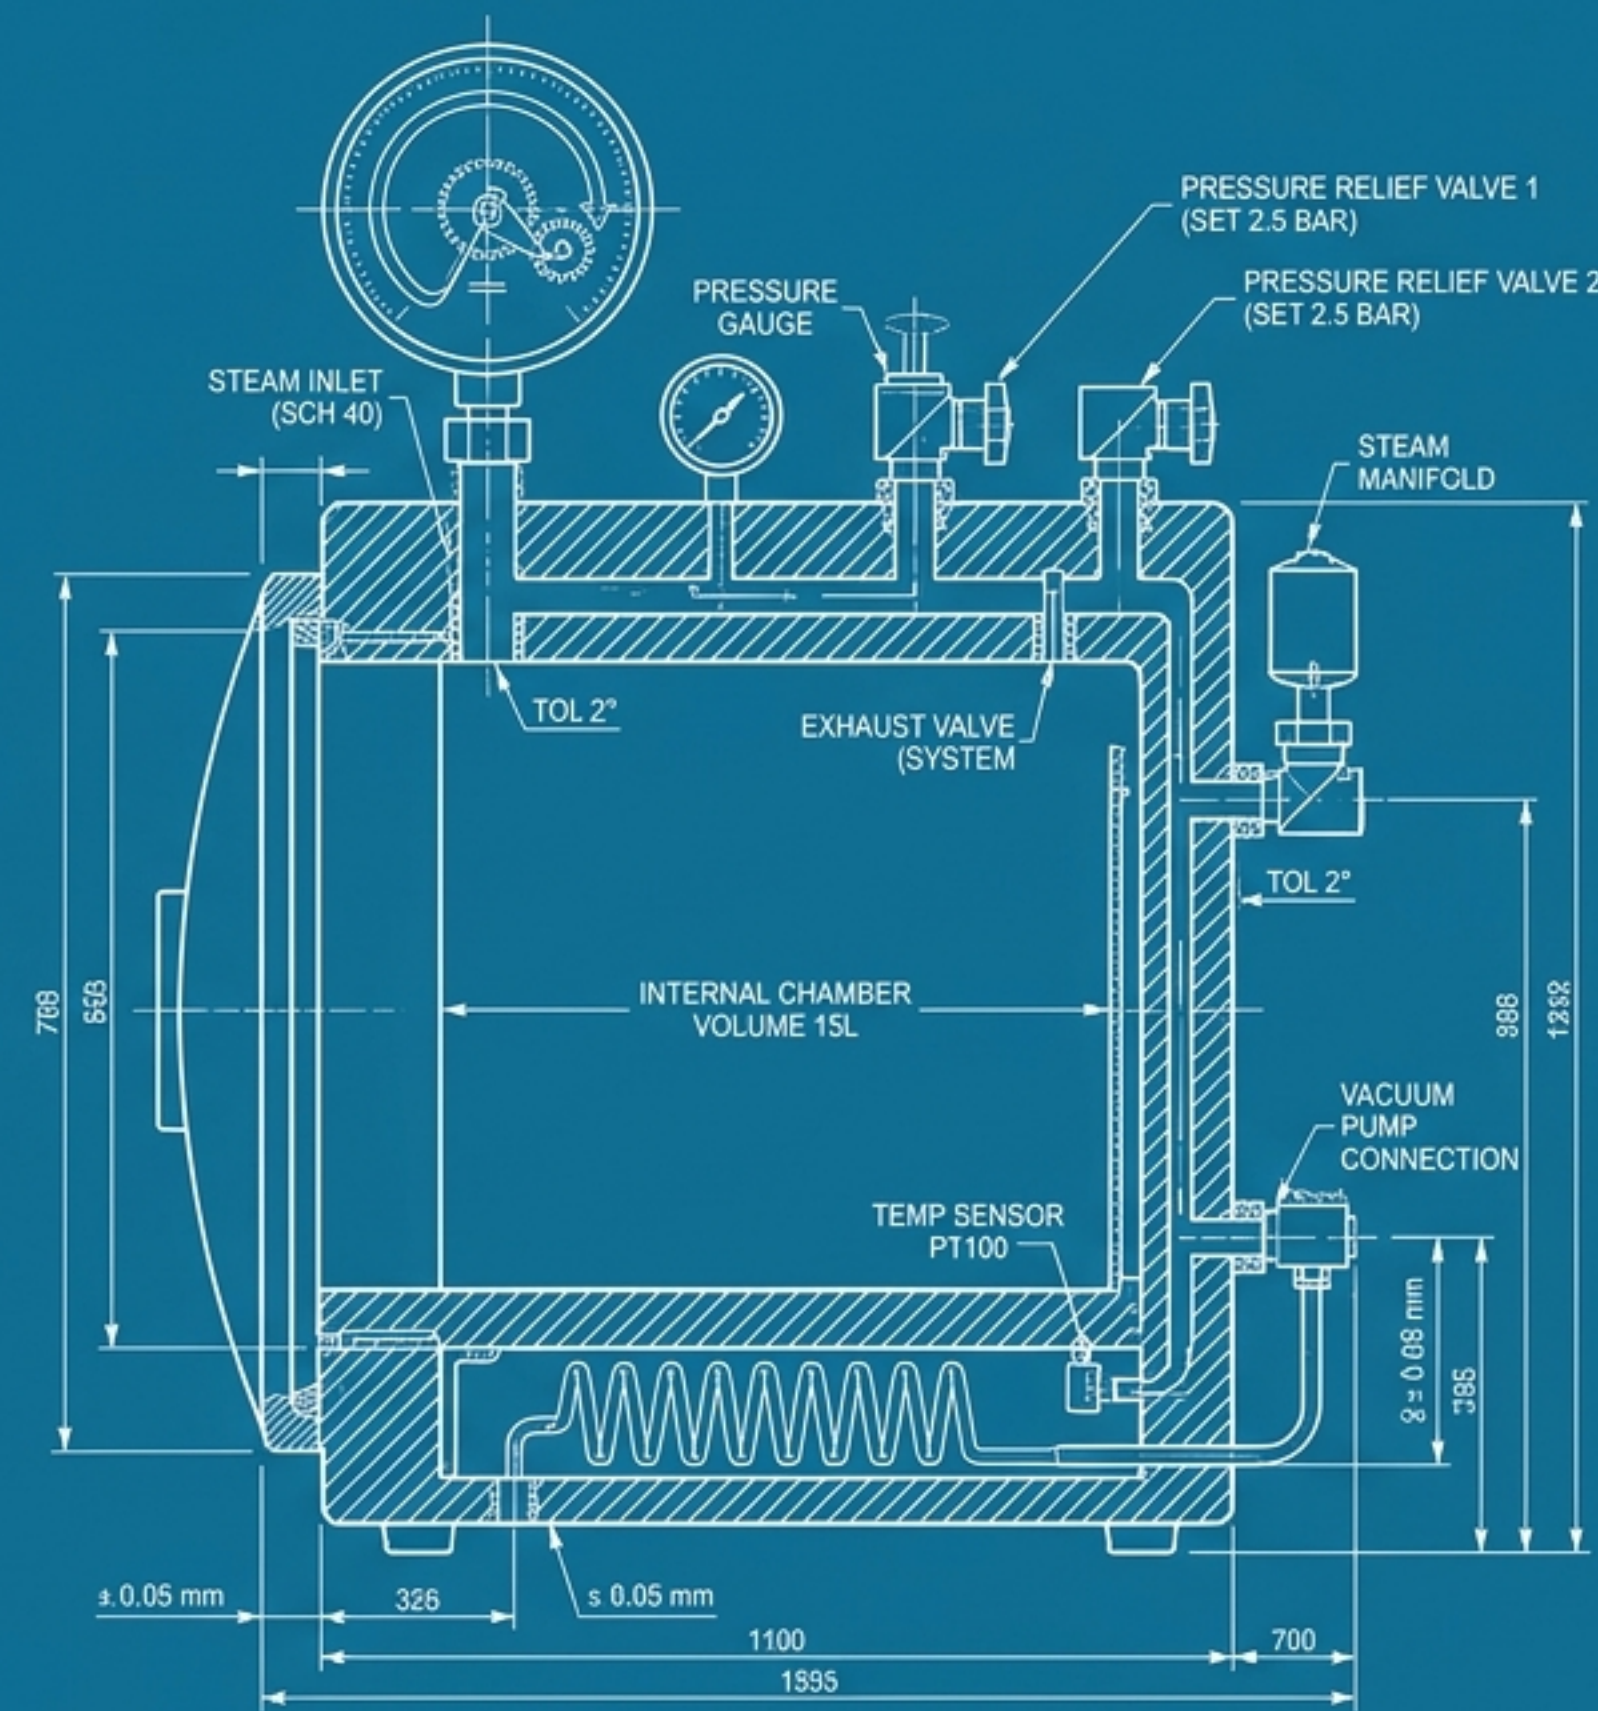

Validated autoclave cycles destroy bloodborne pathogens on reusable equipment.
VERIFY CYCLE PARAMETERS DAILY.