


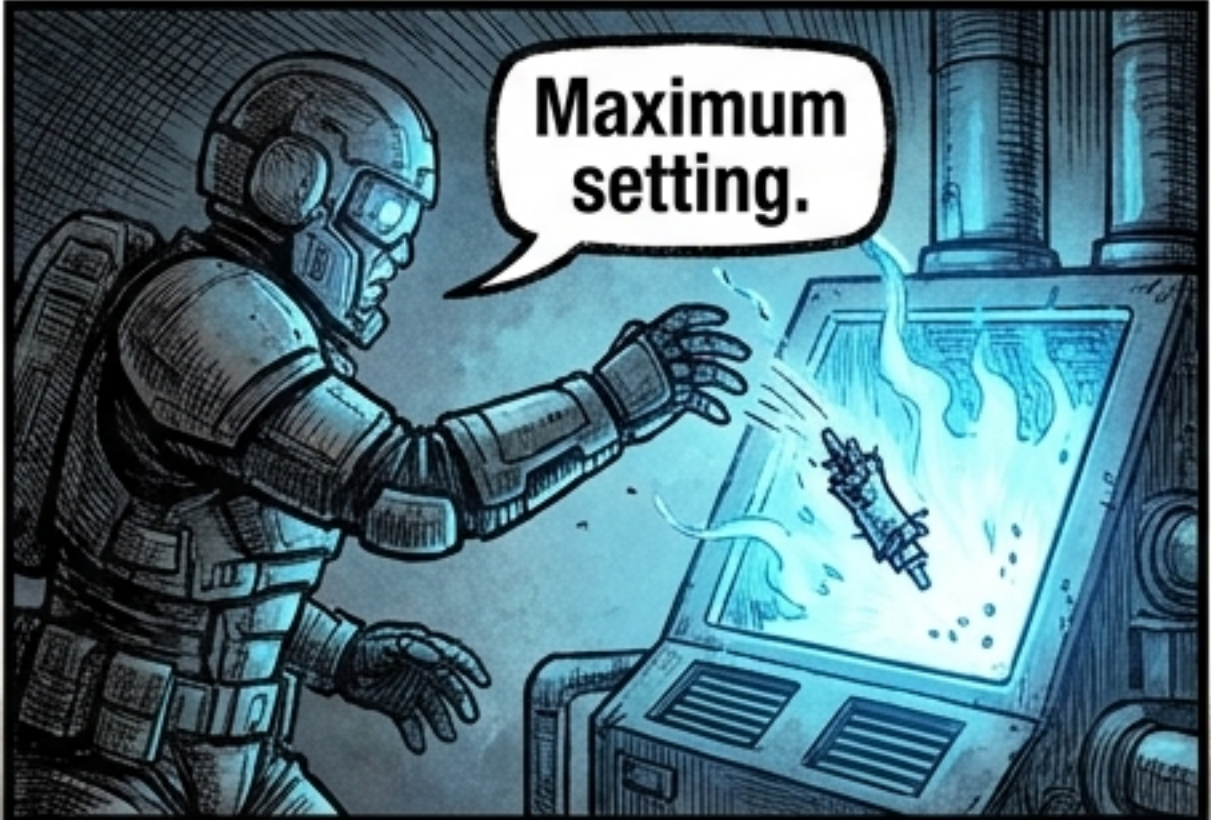

Instruments must be scrubbed completely free of visible residue before effective sterilization can begin.
You cannot have dirty equipment if you no longer have equipment.