


B-Cycle steam sterilizer operating parameters.

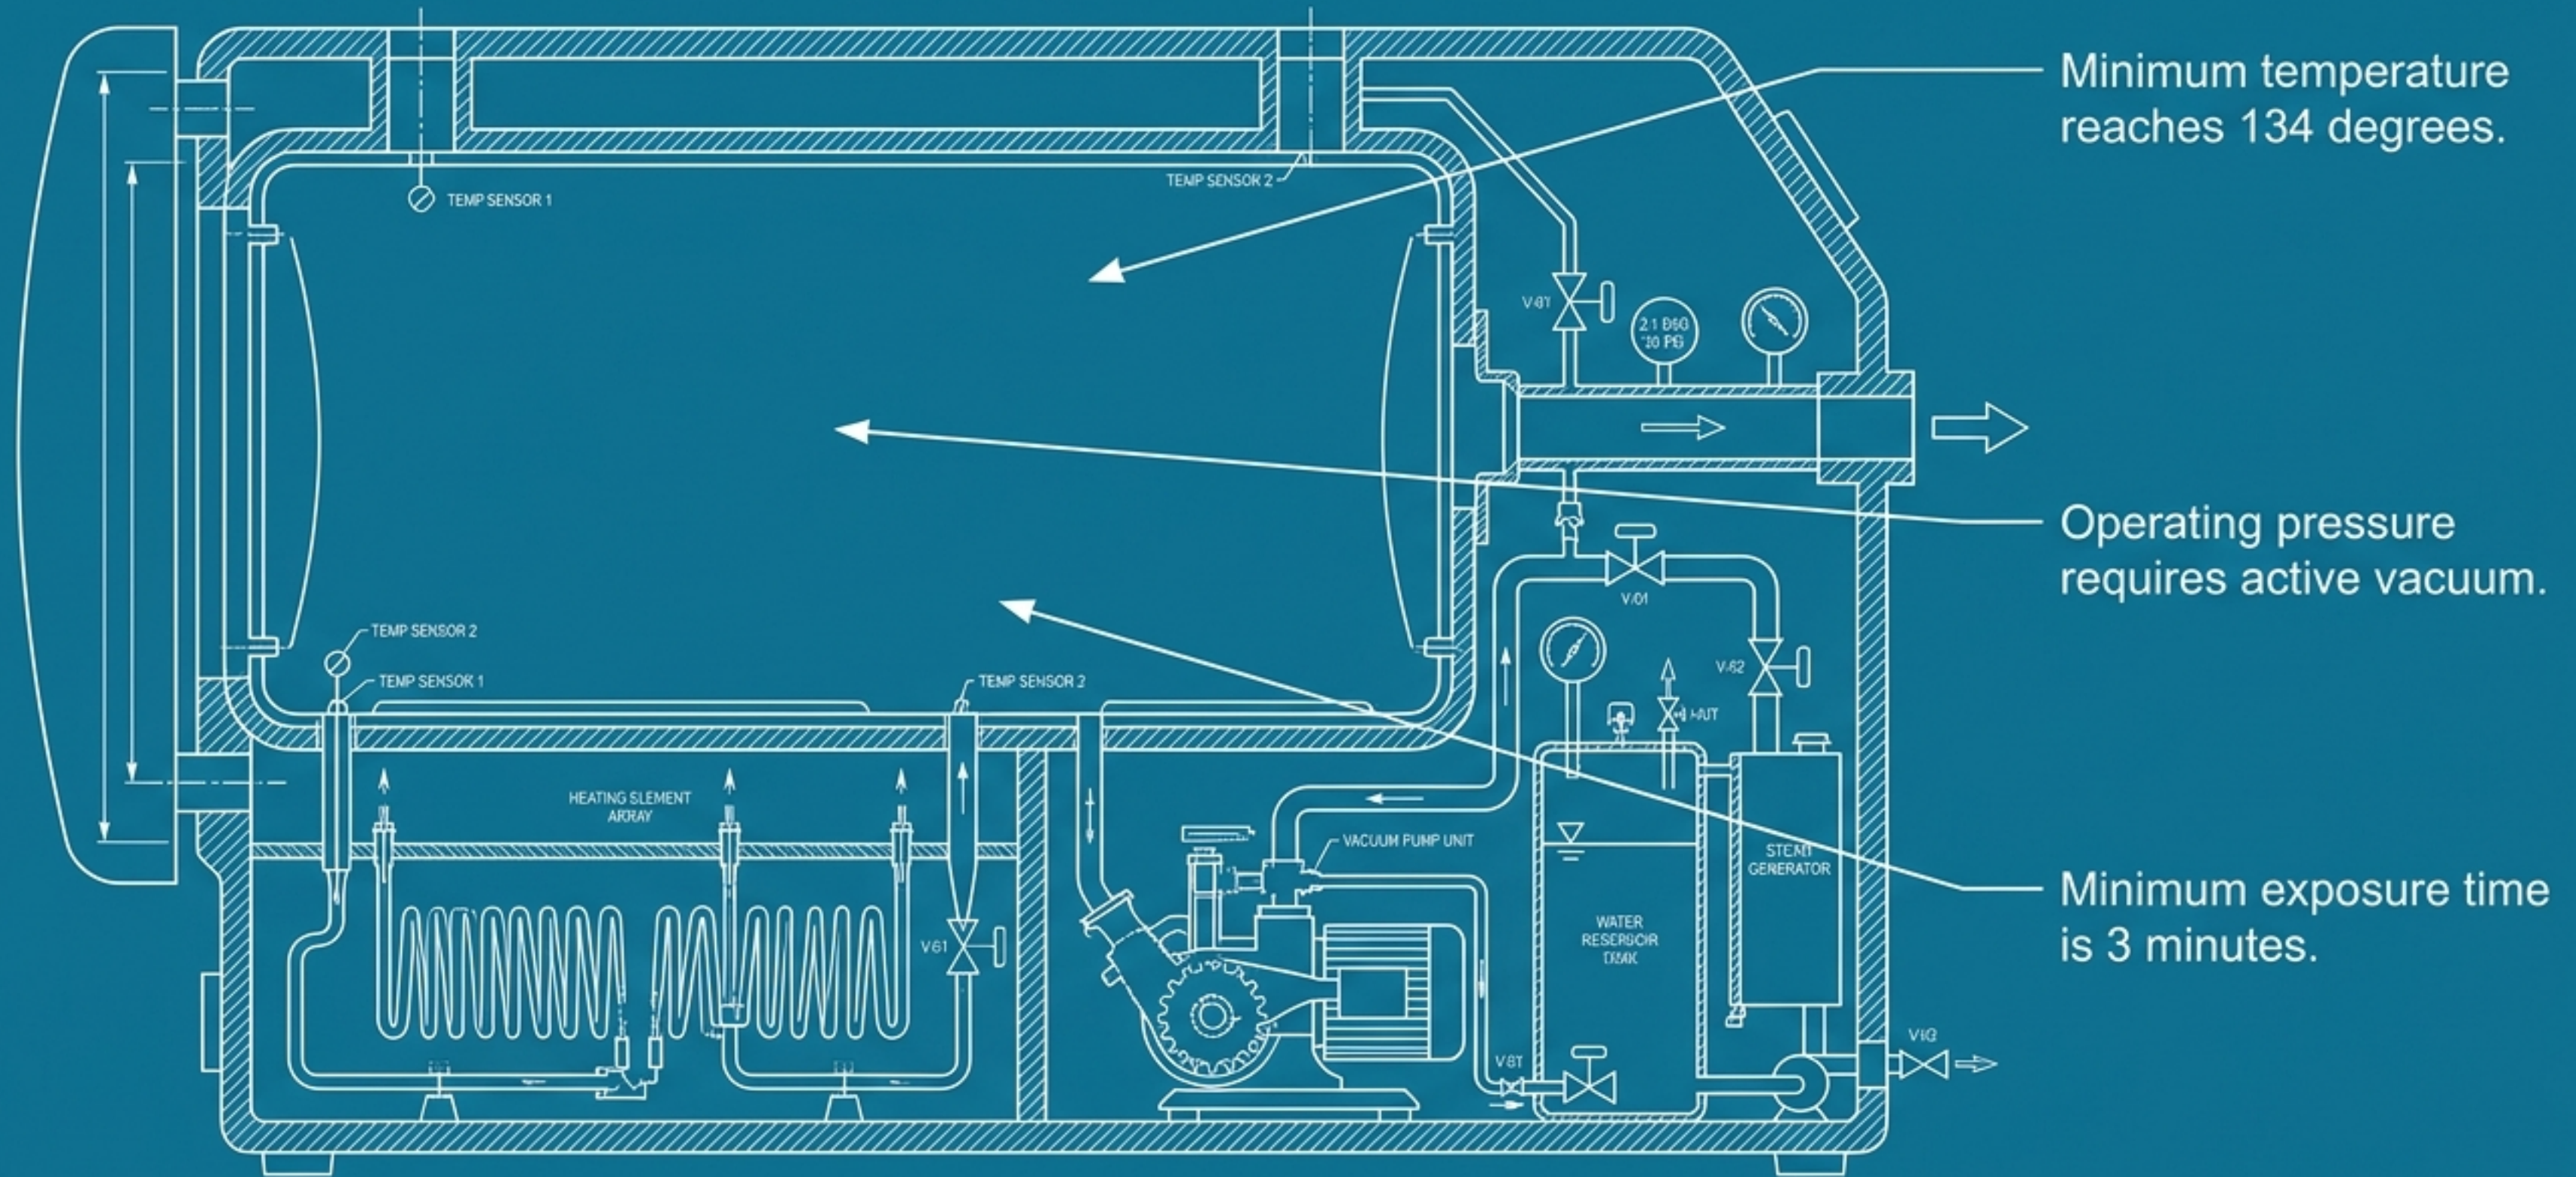

Distilled water conductivity must remain below 5 microsiemens.

VERIFY EVERY STERILIZATION LOAD.