


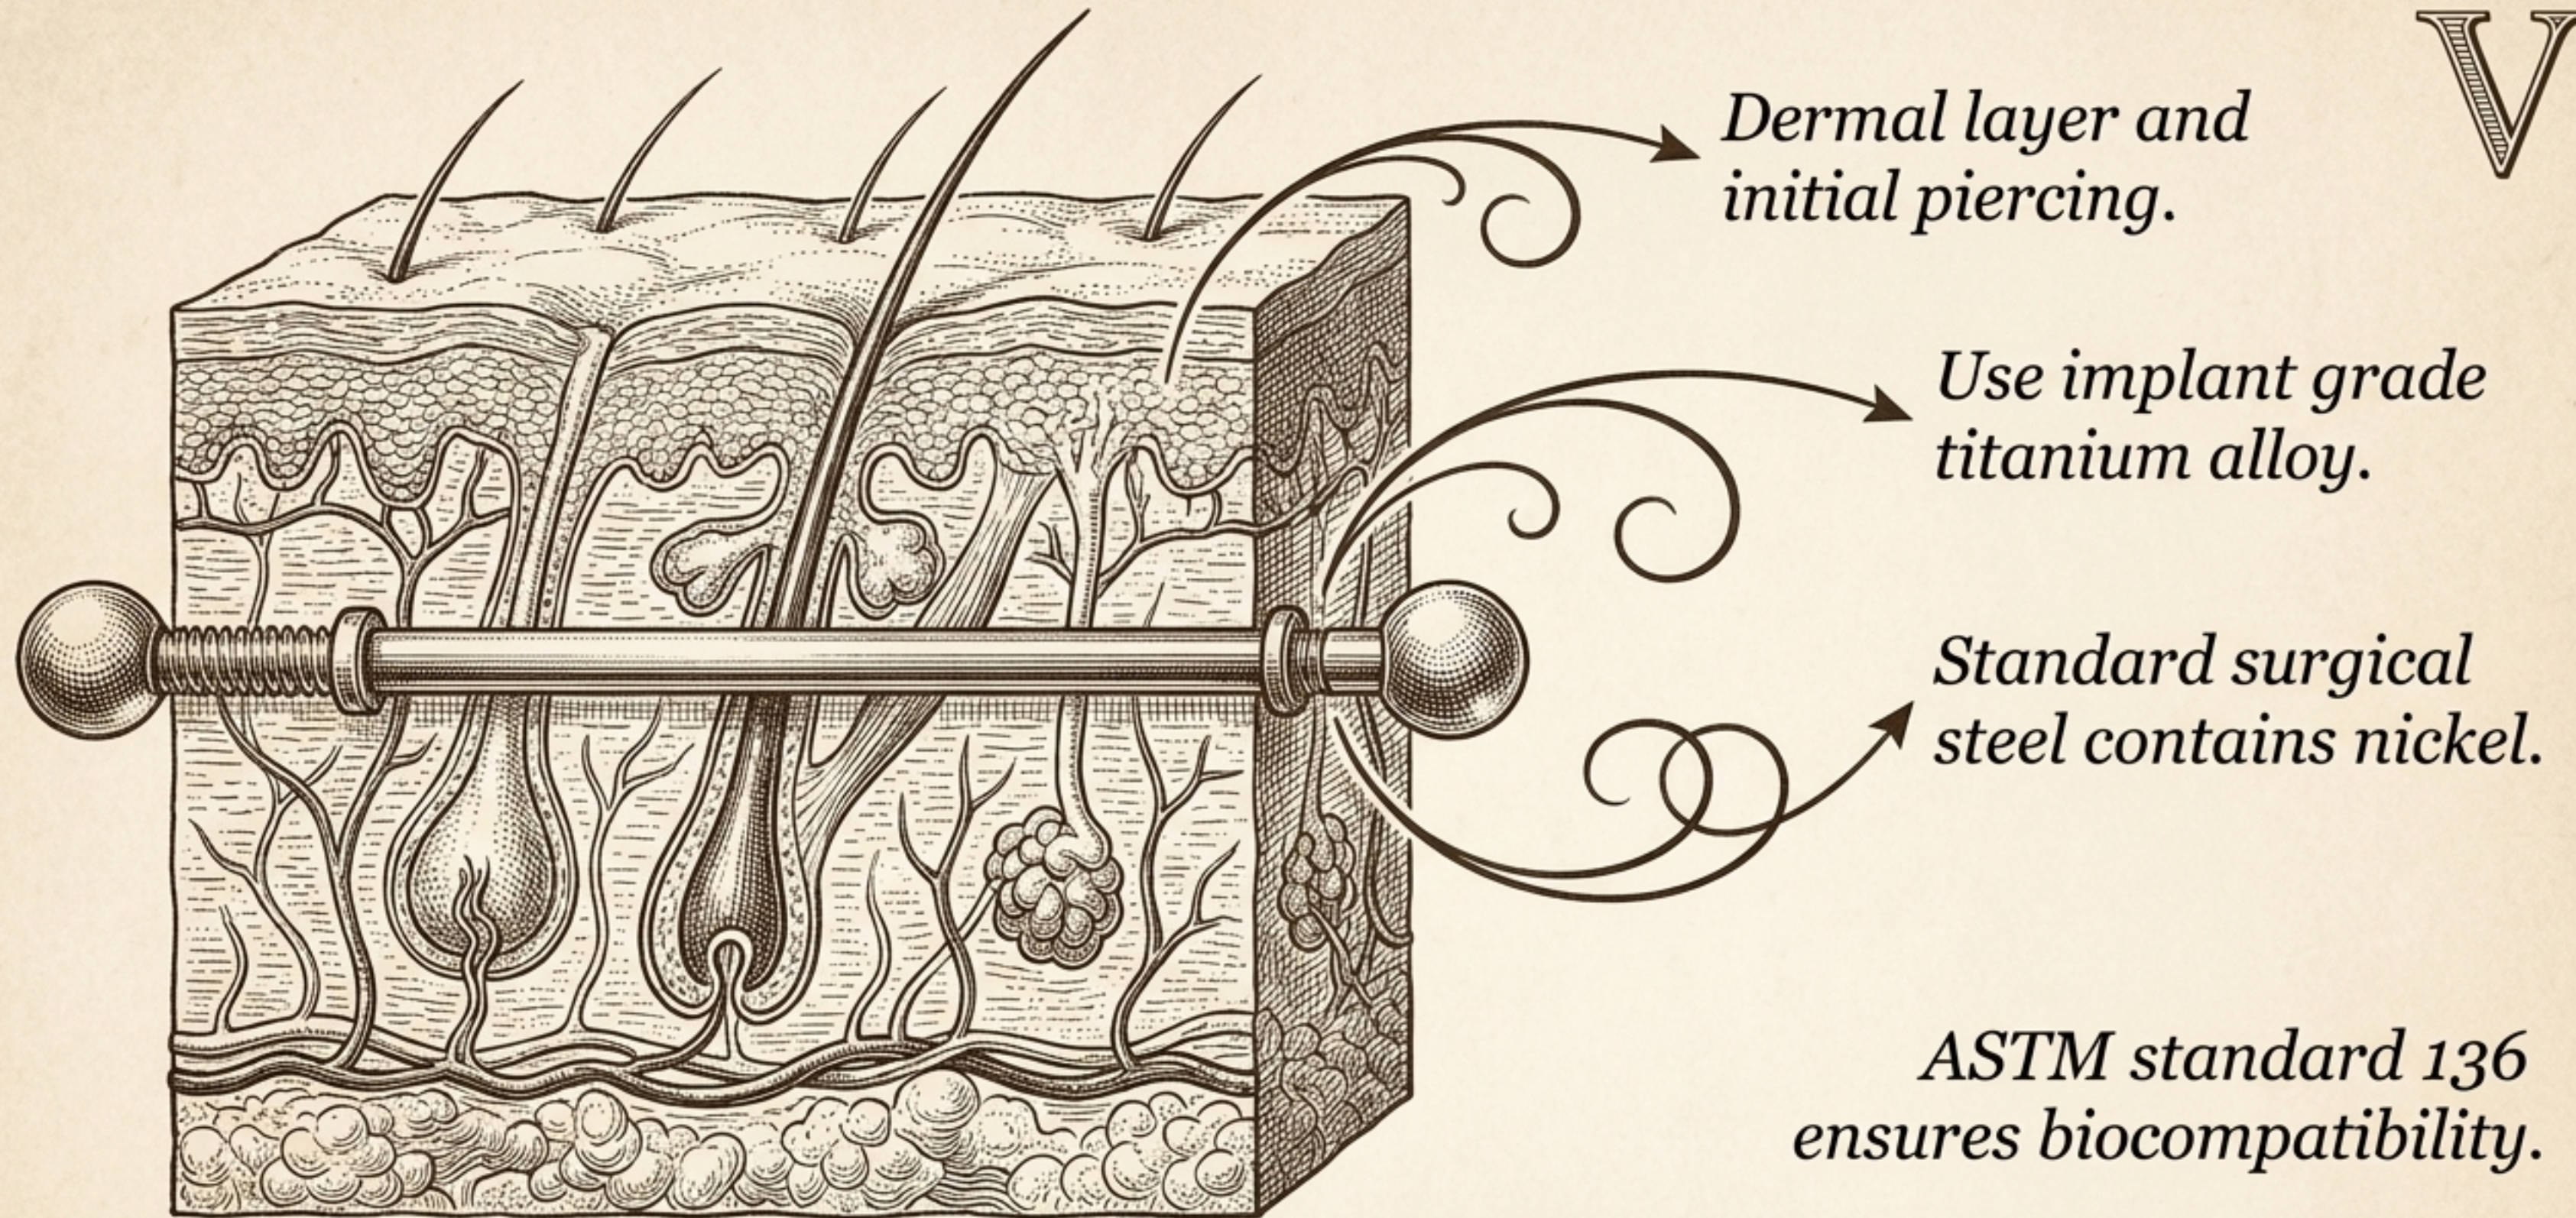

Nickel release must remain below 0.2 micrograms per week.
USE IMPLANT GRADE TITANIUM.