


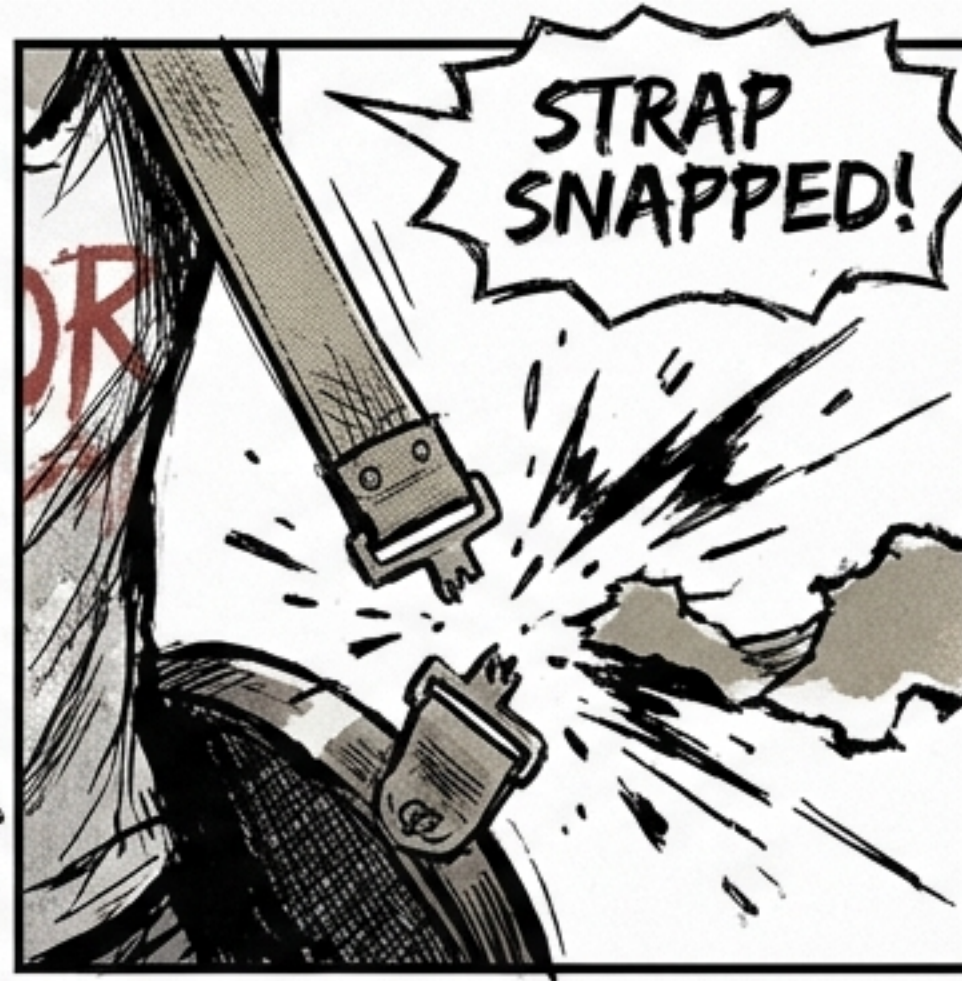

Medical grade silicone has extremely low tear strength and is highly unsuitable for threaded jewelry components.
The silicone post failed instantly as a heavy guitar strap.