


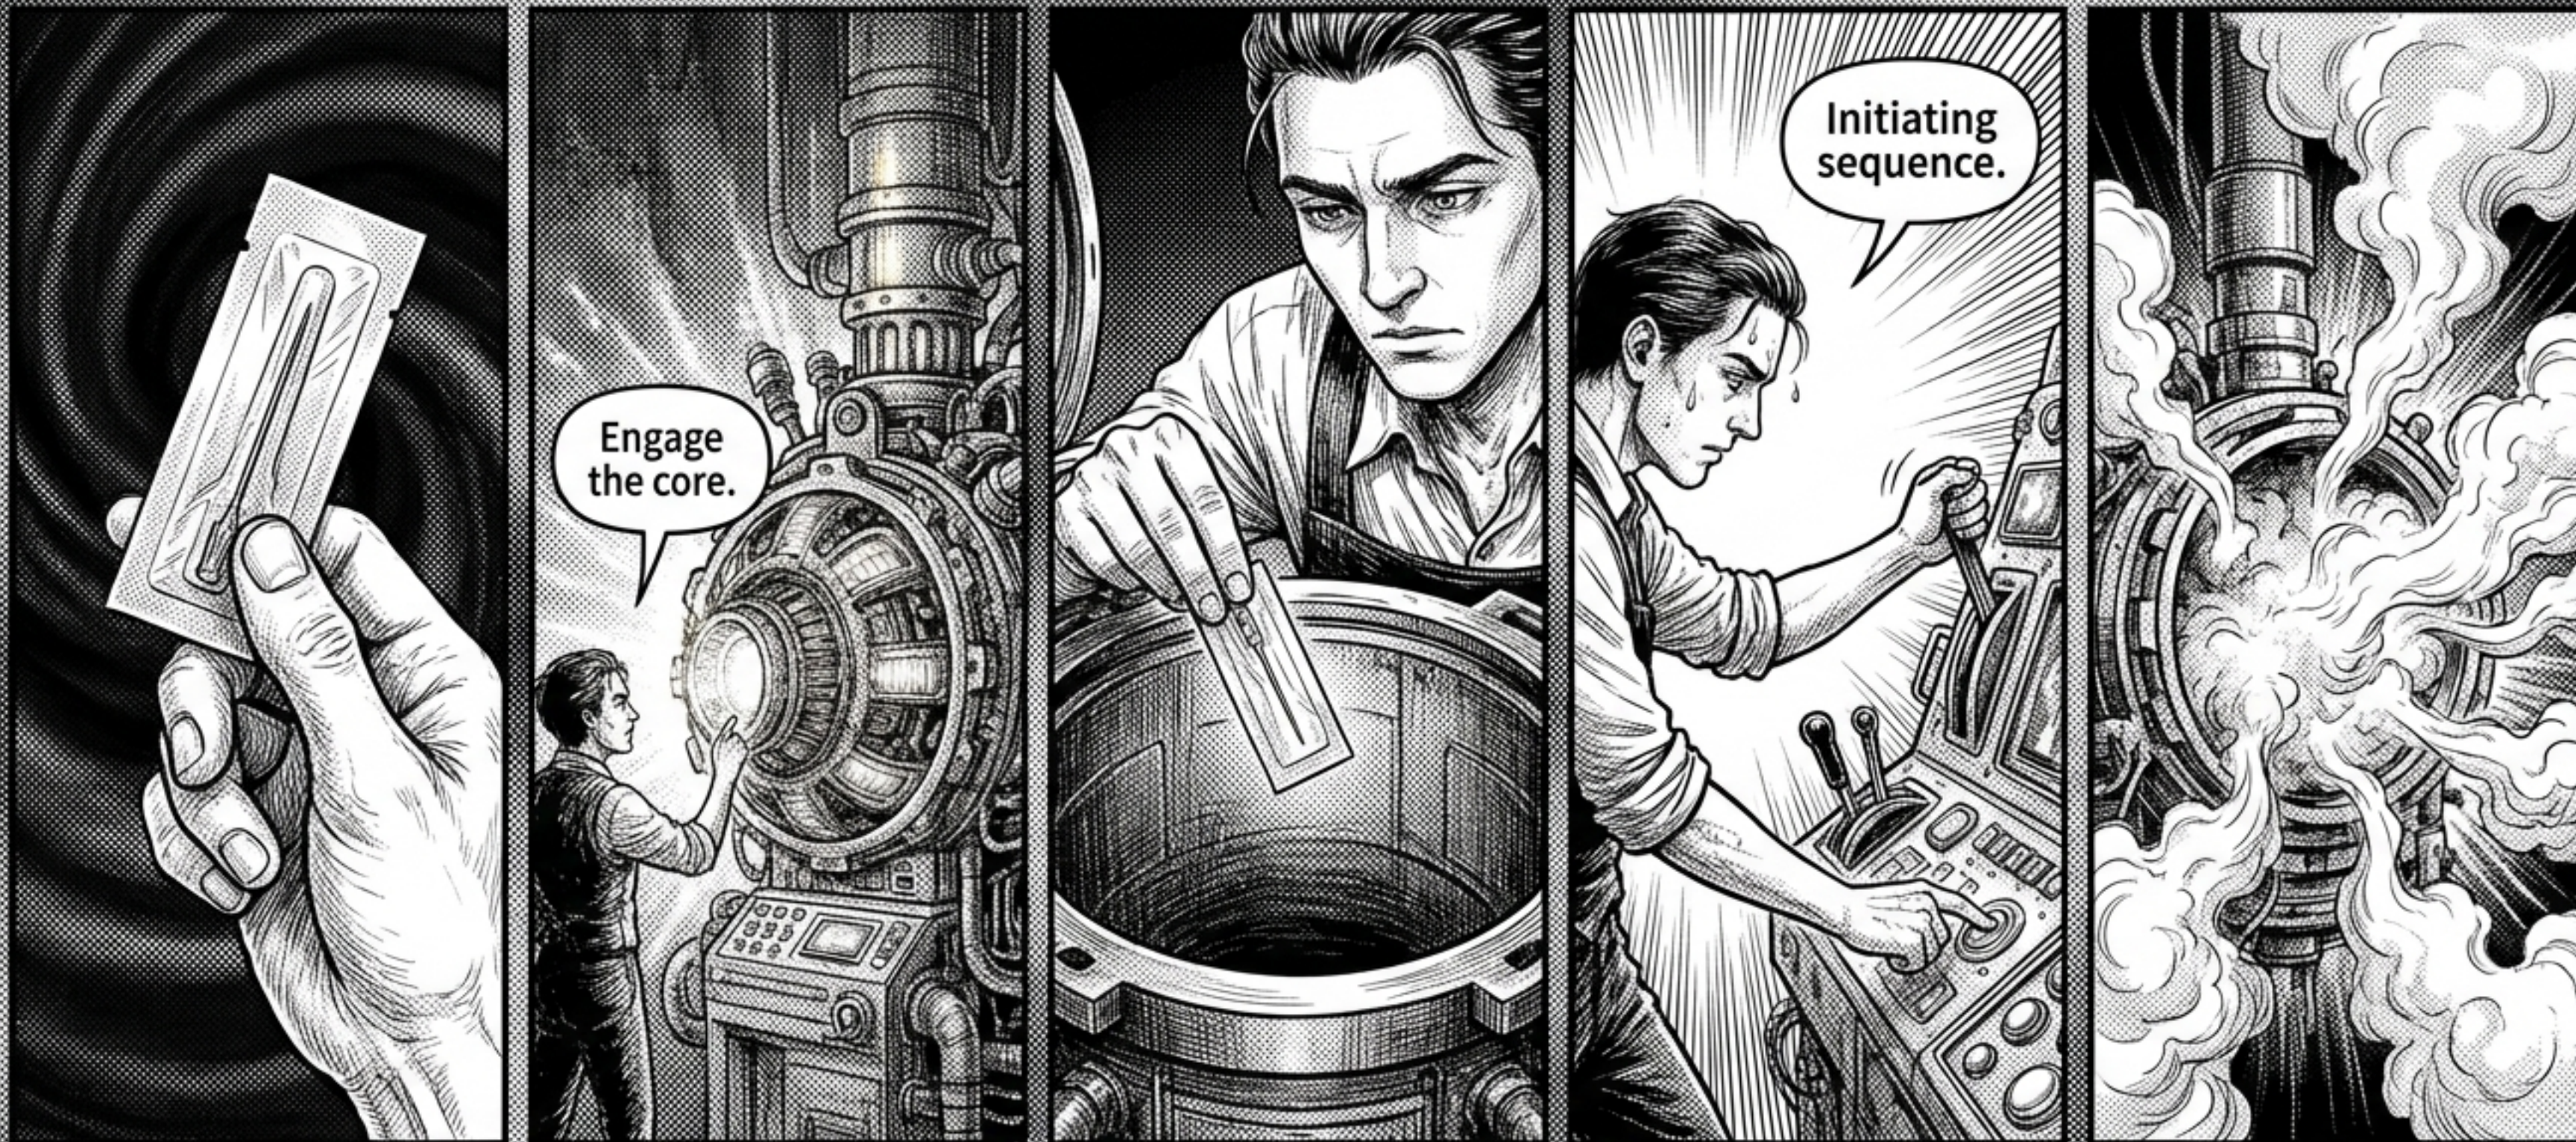

Reusable procedure instruments must be thoroughly cleaned, individually packaged, and sterilized in a steam autoclave.
Deploying maximum thermal pressure for a tiny piece of metal