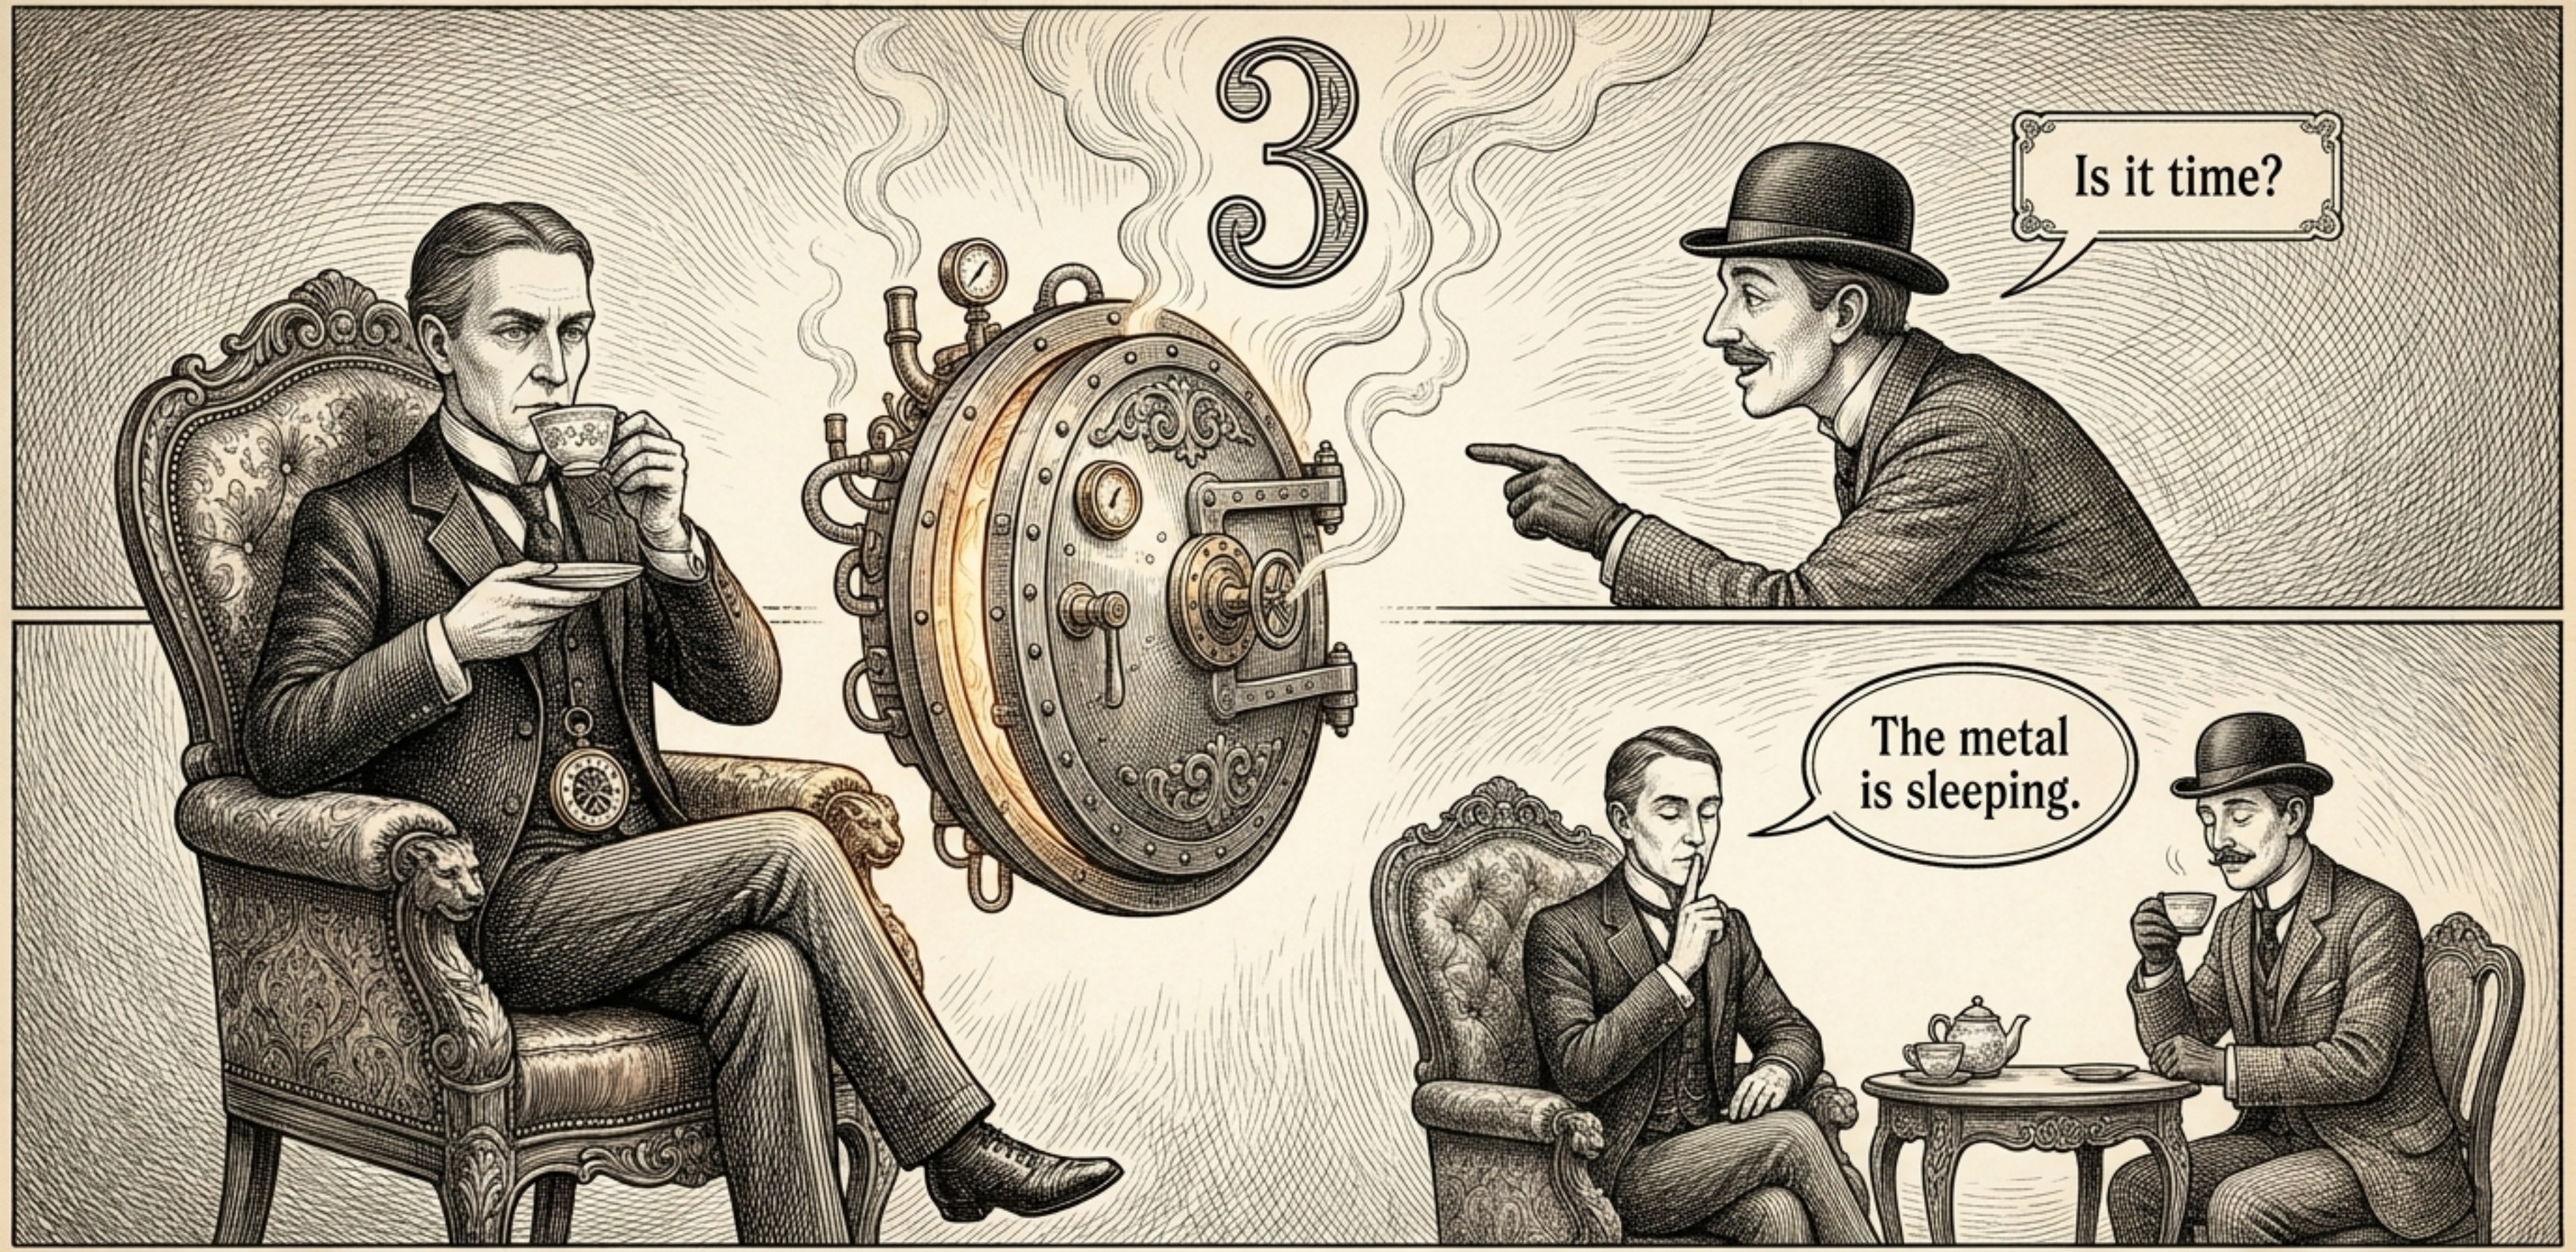

Instruments should be used up to 3 hours after the sterilisation cycle is finished when the door remains shut.

Perfection cannot be rushed but it does expire shortly after lunch.