


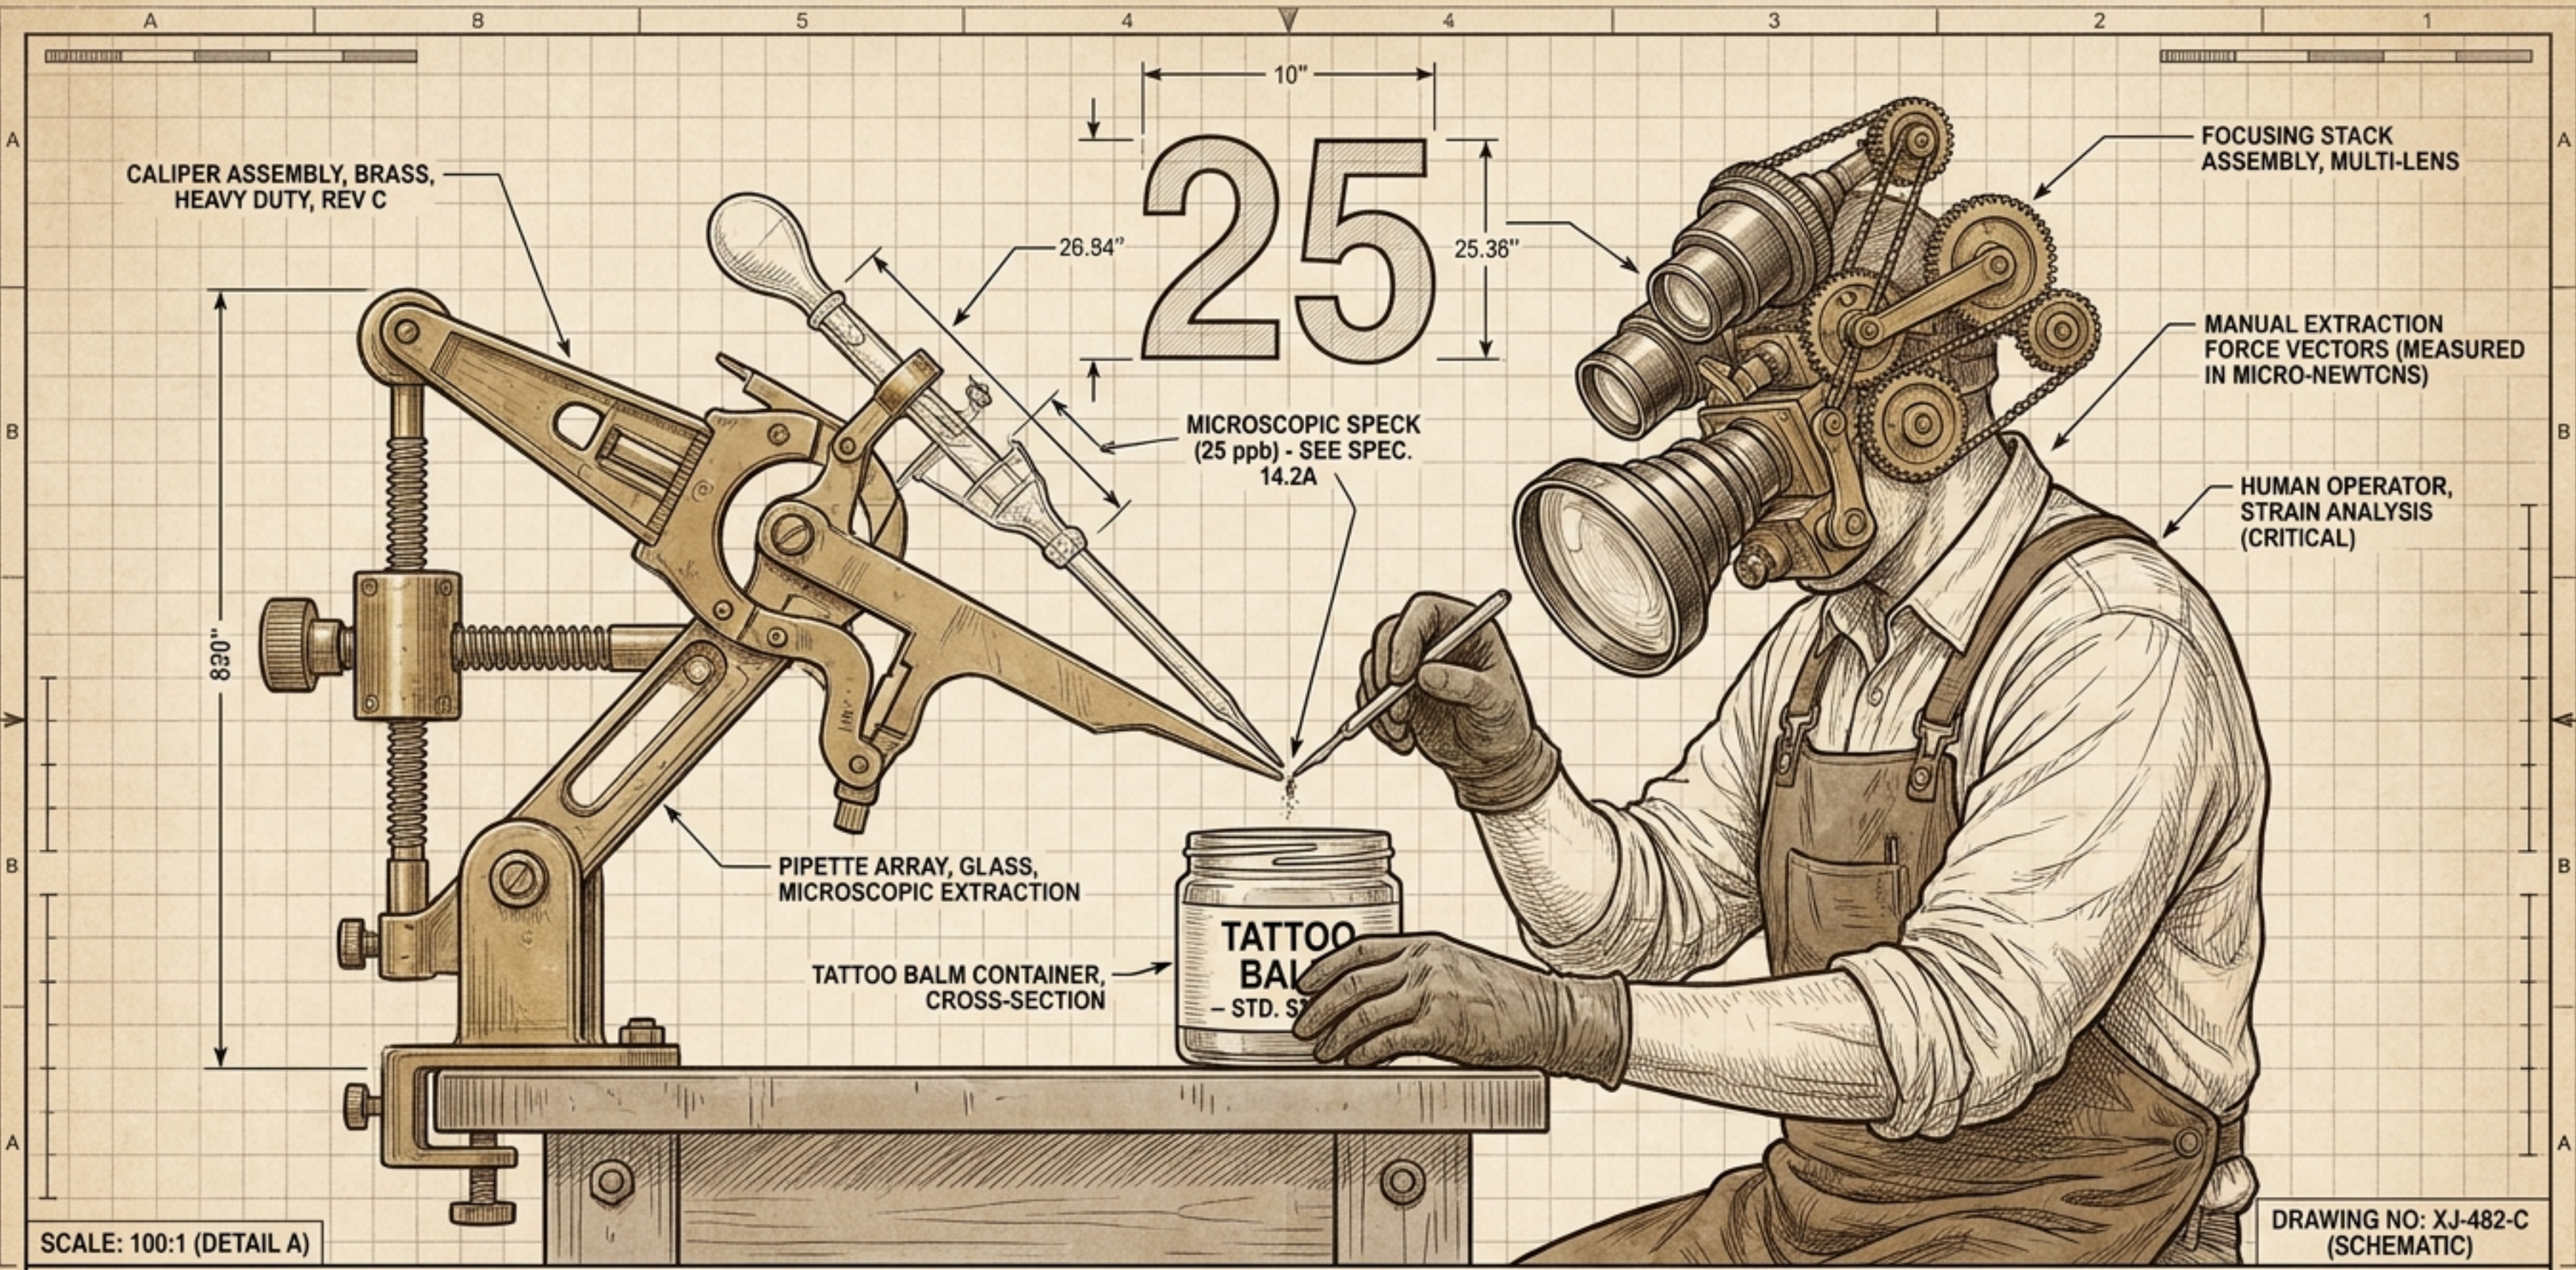

A product may not contain 25 ppb or more of PFHxA and its salts.

The laboratory calibration takes longer than the backpiece.