


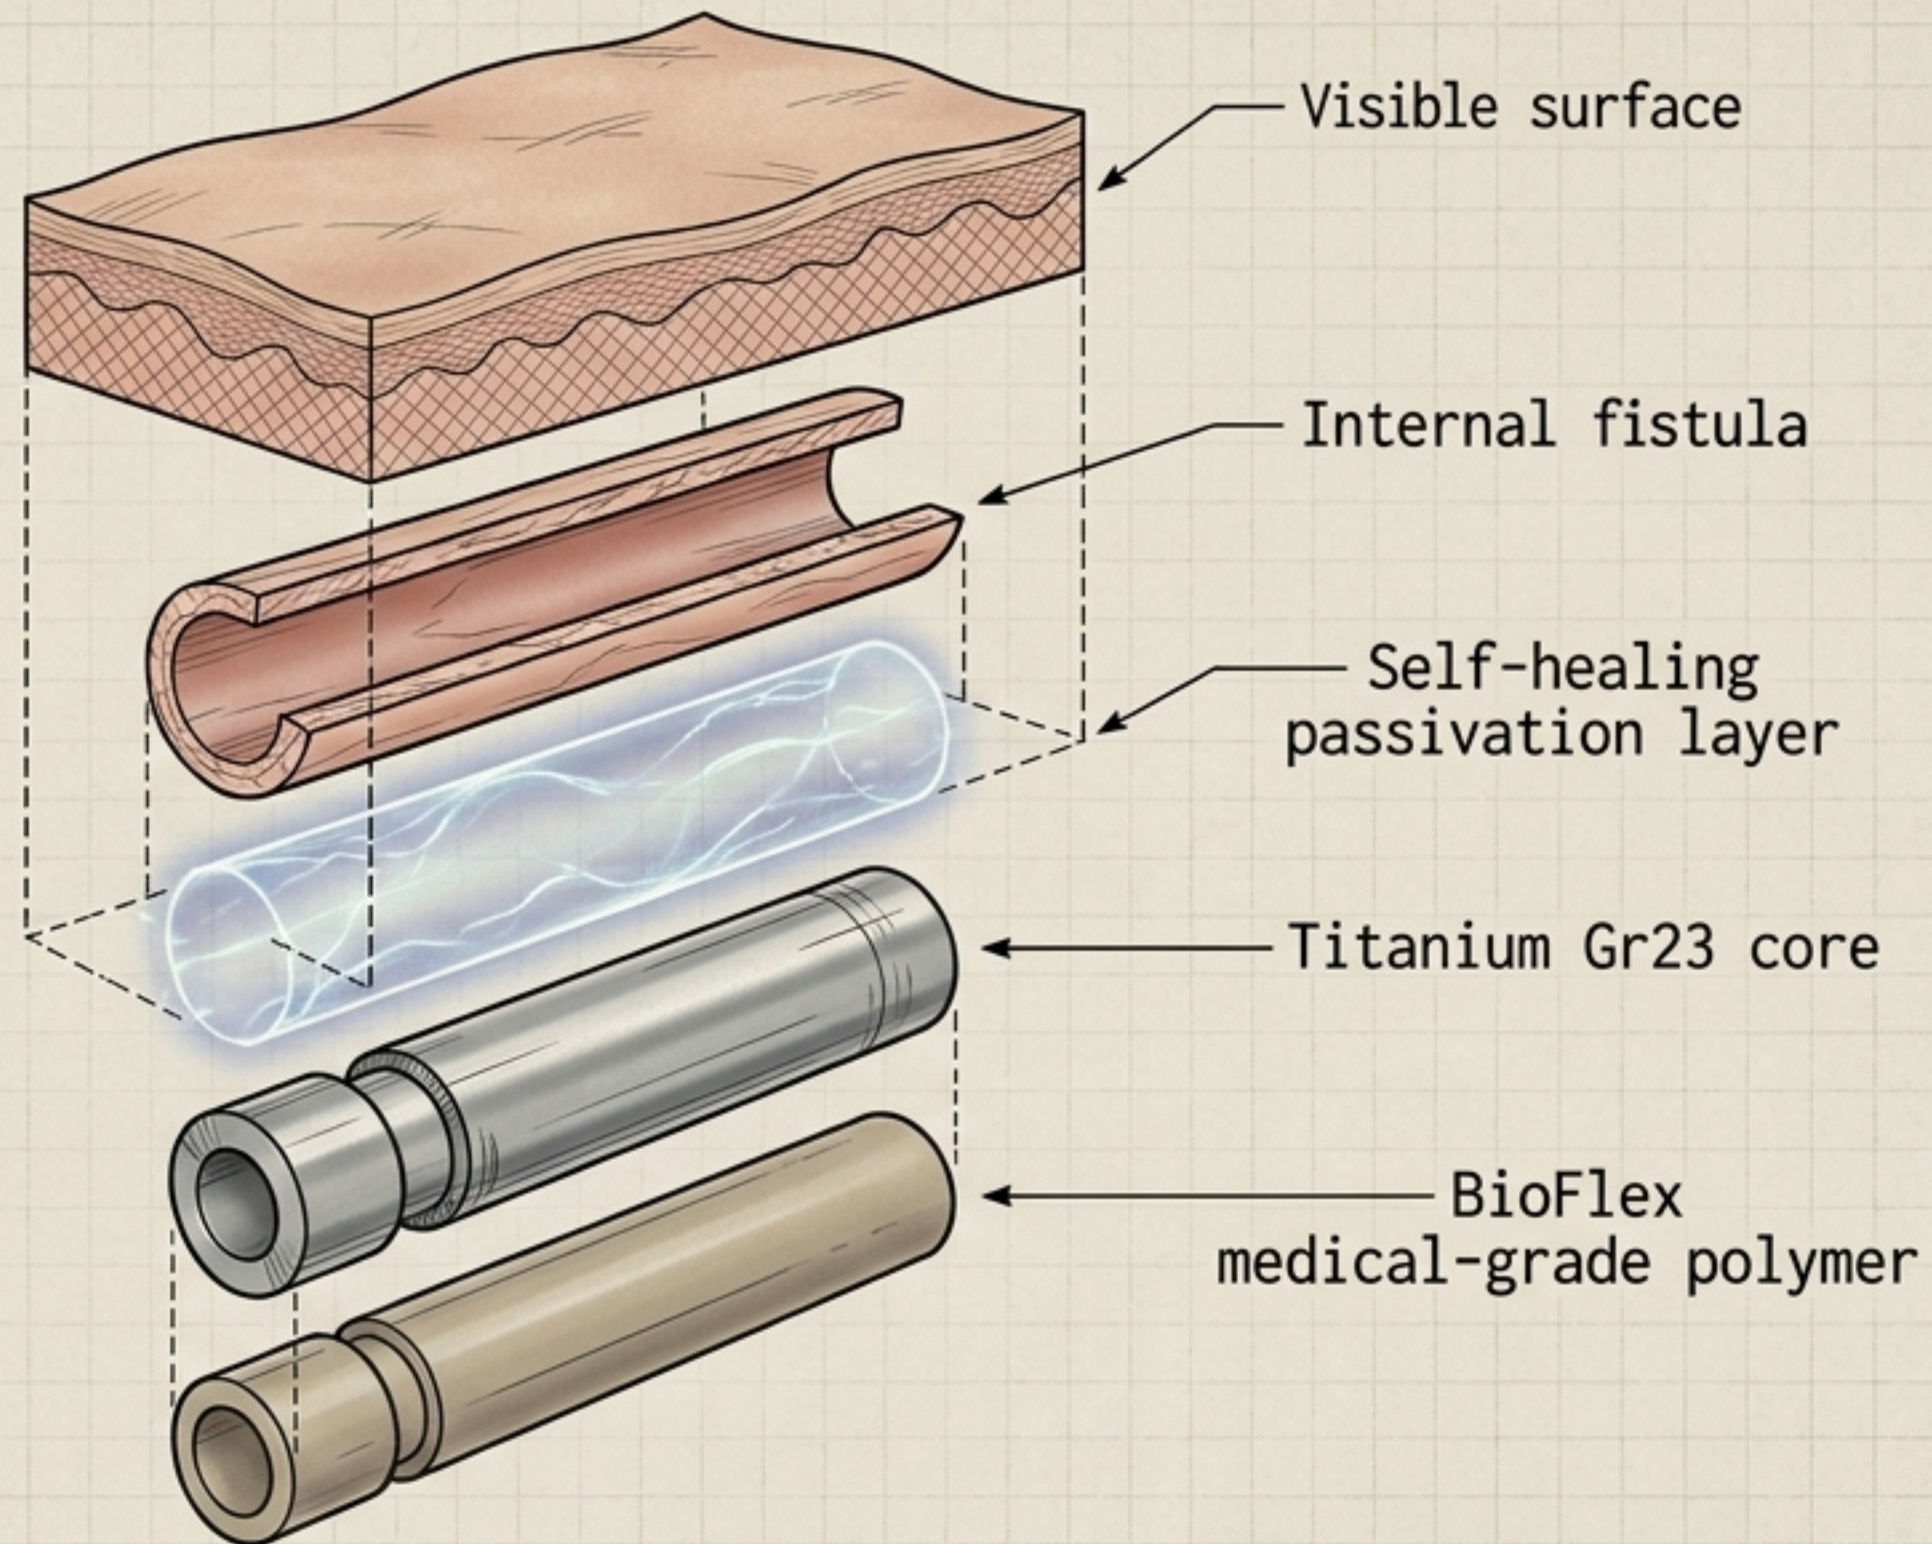

Only highly biocompatible materials can safely maintain an open fistula for long-term wear.

START WITH WHAT IS SAFE.