
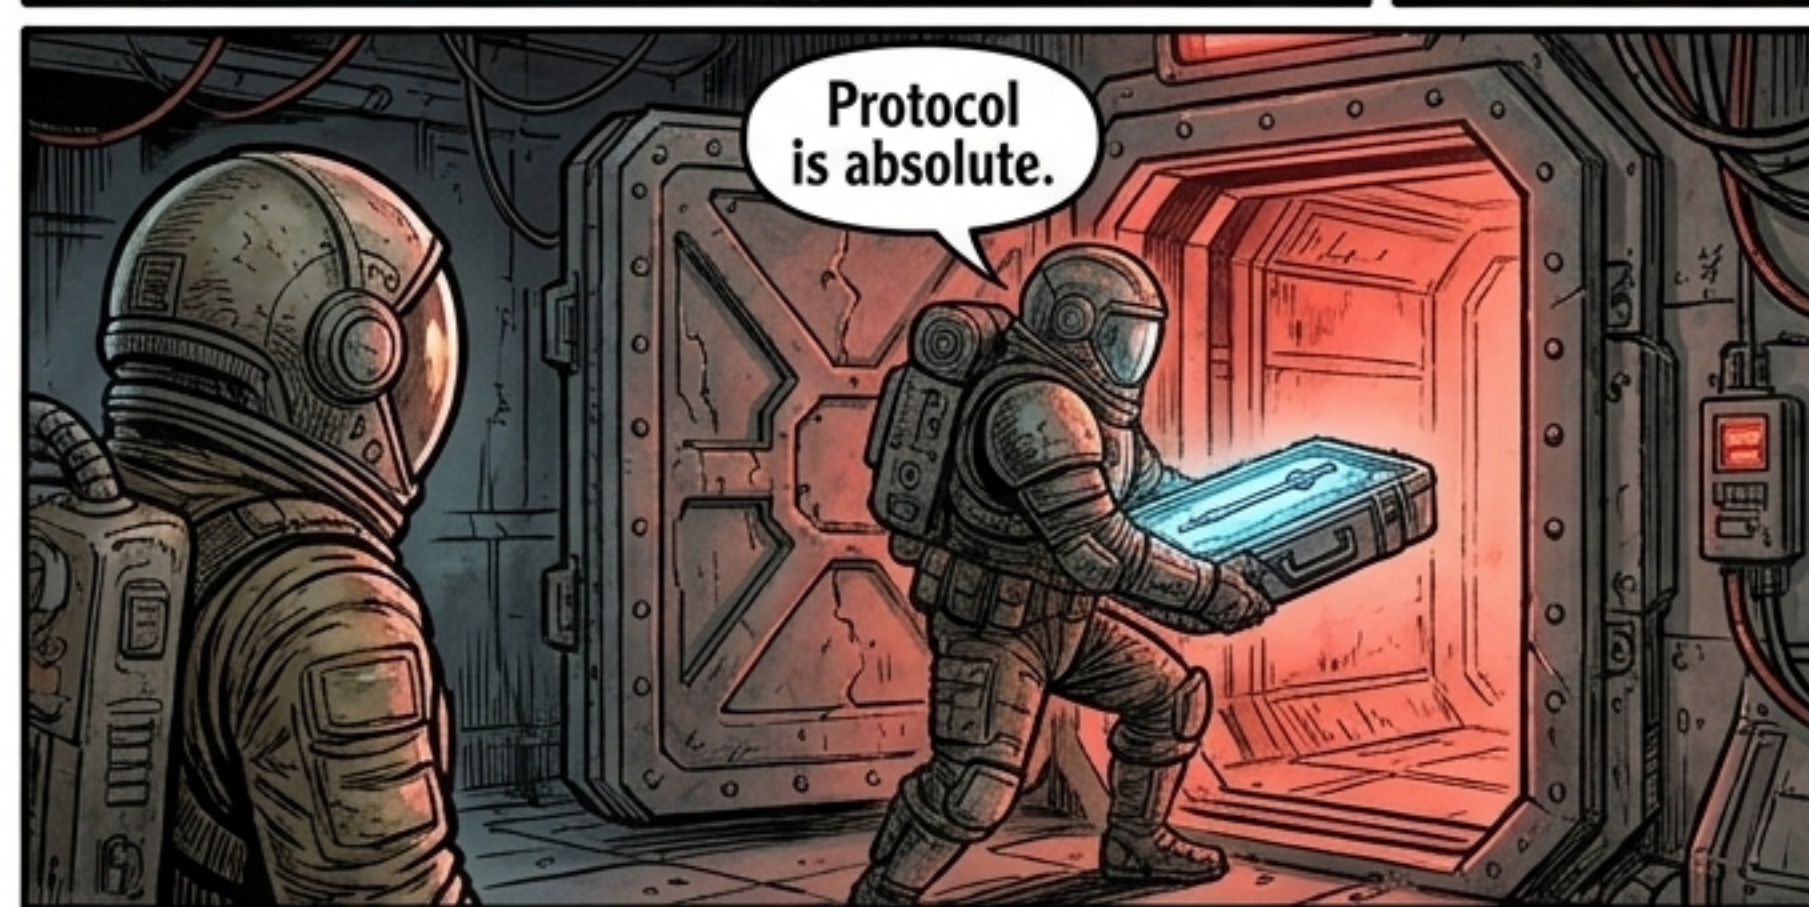


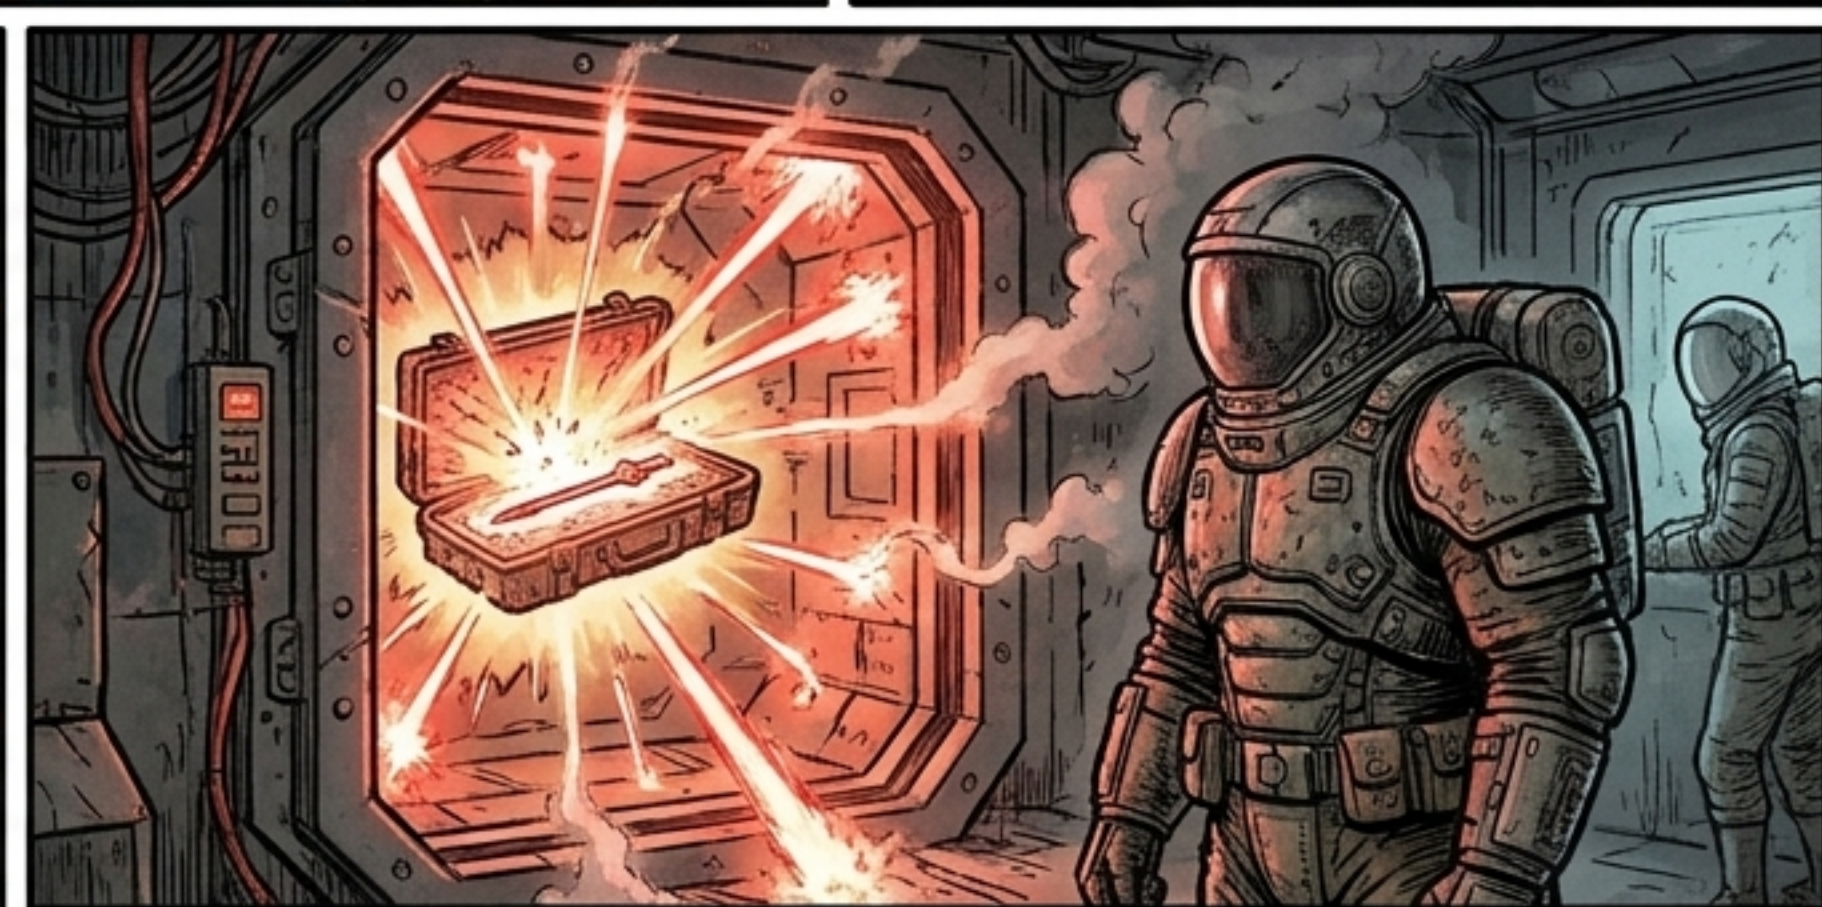

Any opened package containing sterile material that remains unused must undergo the complete decontamination process again.
The airlock cares not for changes of heart.