


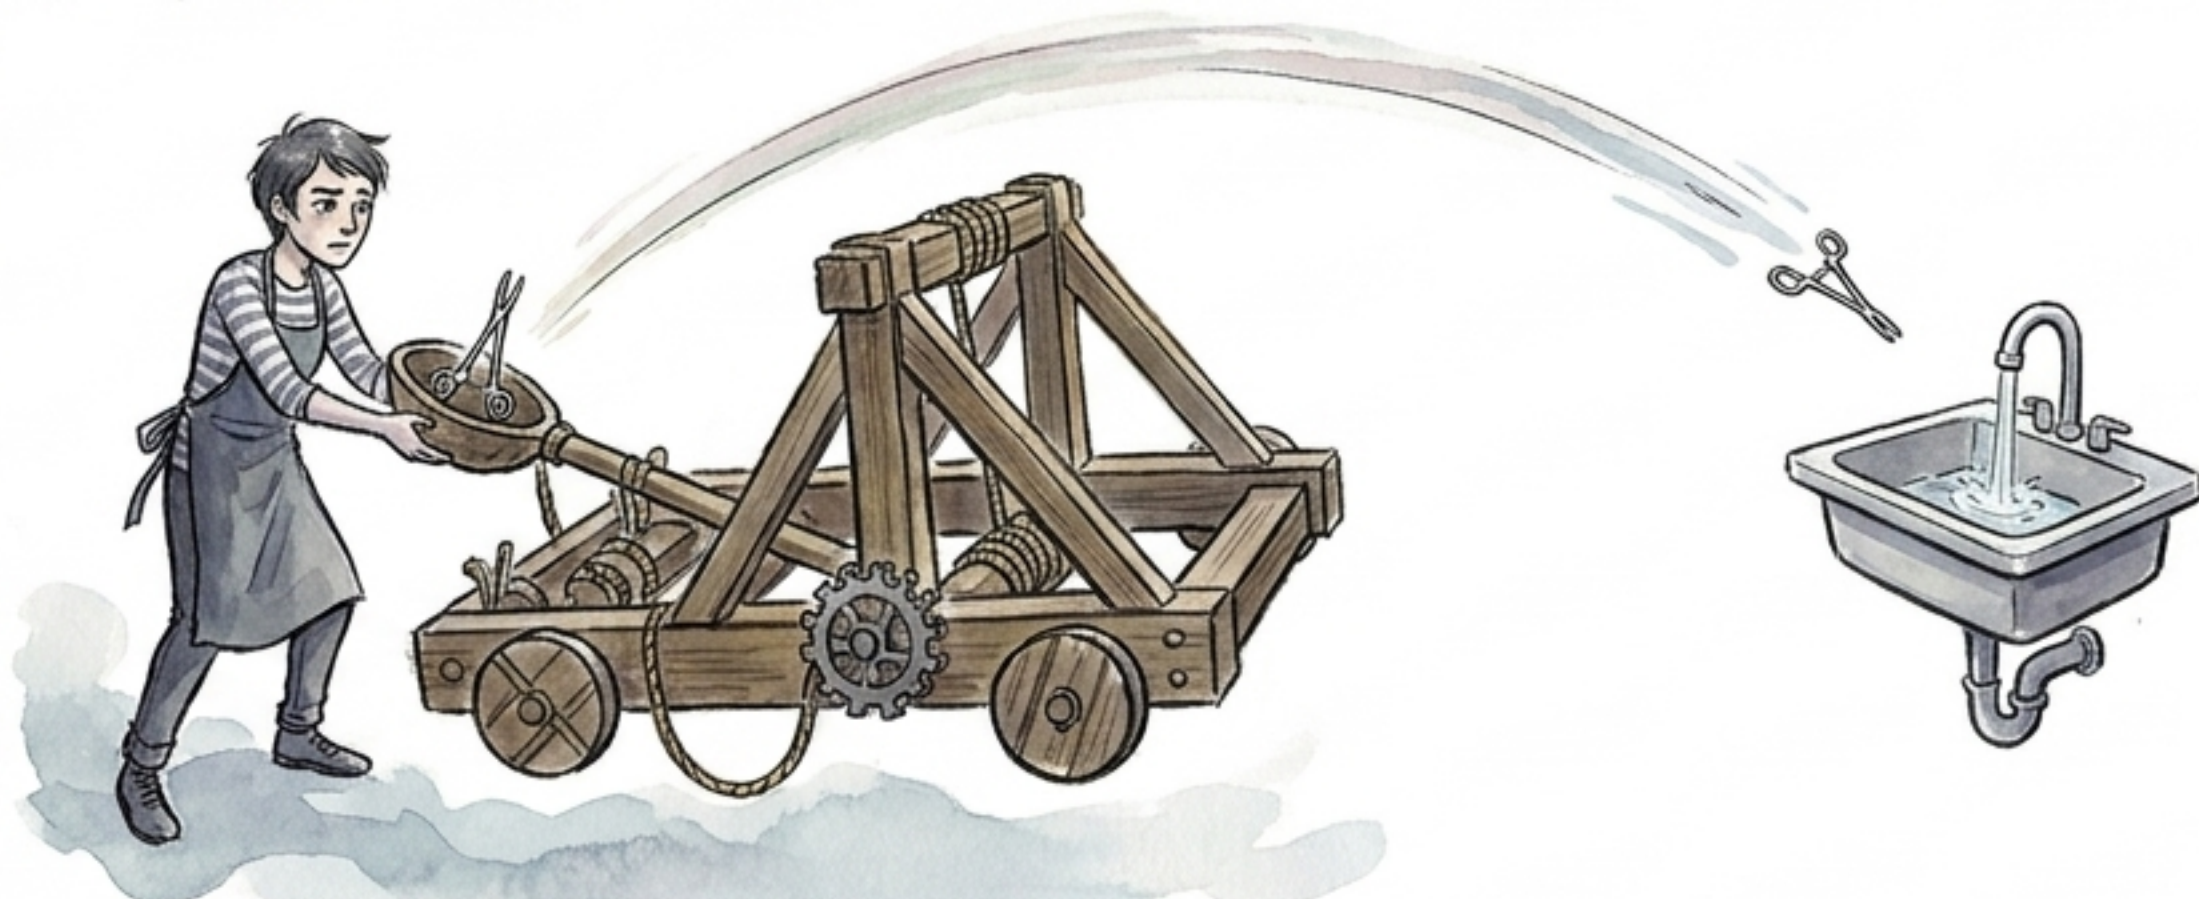

If a sterile tool package is opened but the instrument is not used, it must undergo the entire decontamination and sterilization cycle again.
Return to the starting line.