


STANDARD EN 13060 REQUIRED.
MAXIMUM DRY STORAGE 3 HOURS.
MAXIMUM STERILE SHELF 2 MONTHS.

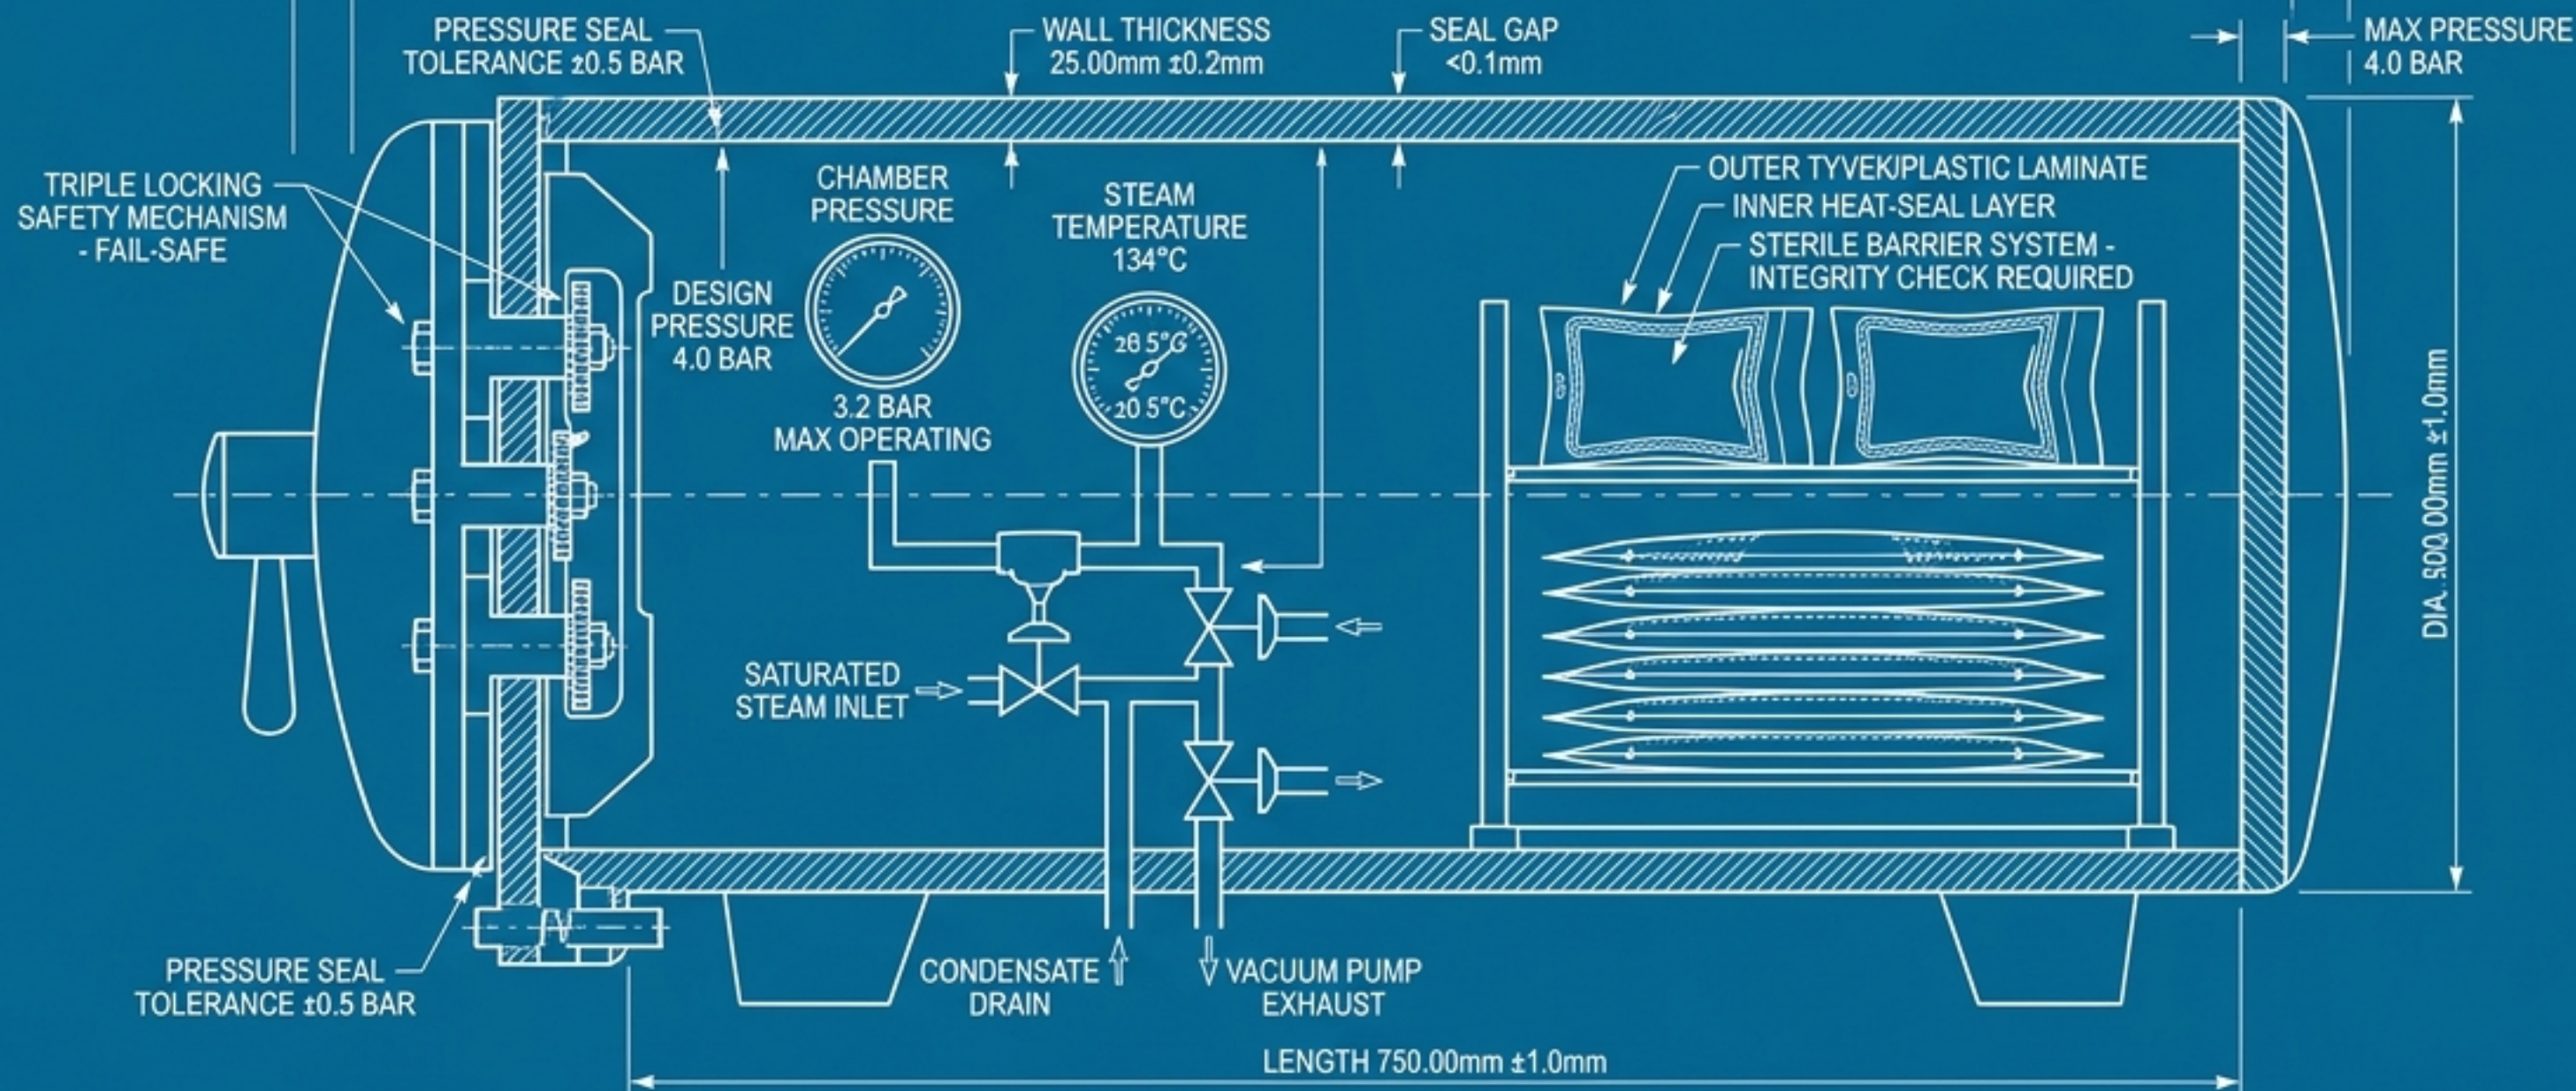

PRECISE PHYSICAL PARAMETERS GOVERN THE LEGAL LIMITS OF INSTRUMENT STERILITY AND STORAGE.
RESPECT TIME AND TEMPERATURE TOLERANCES