




**Run 1
biological
test.**

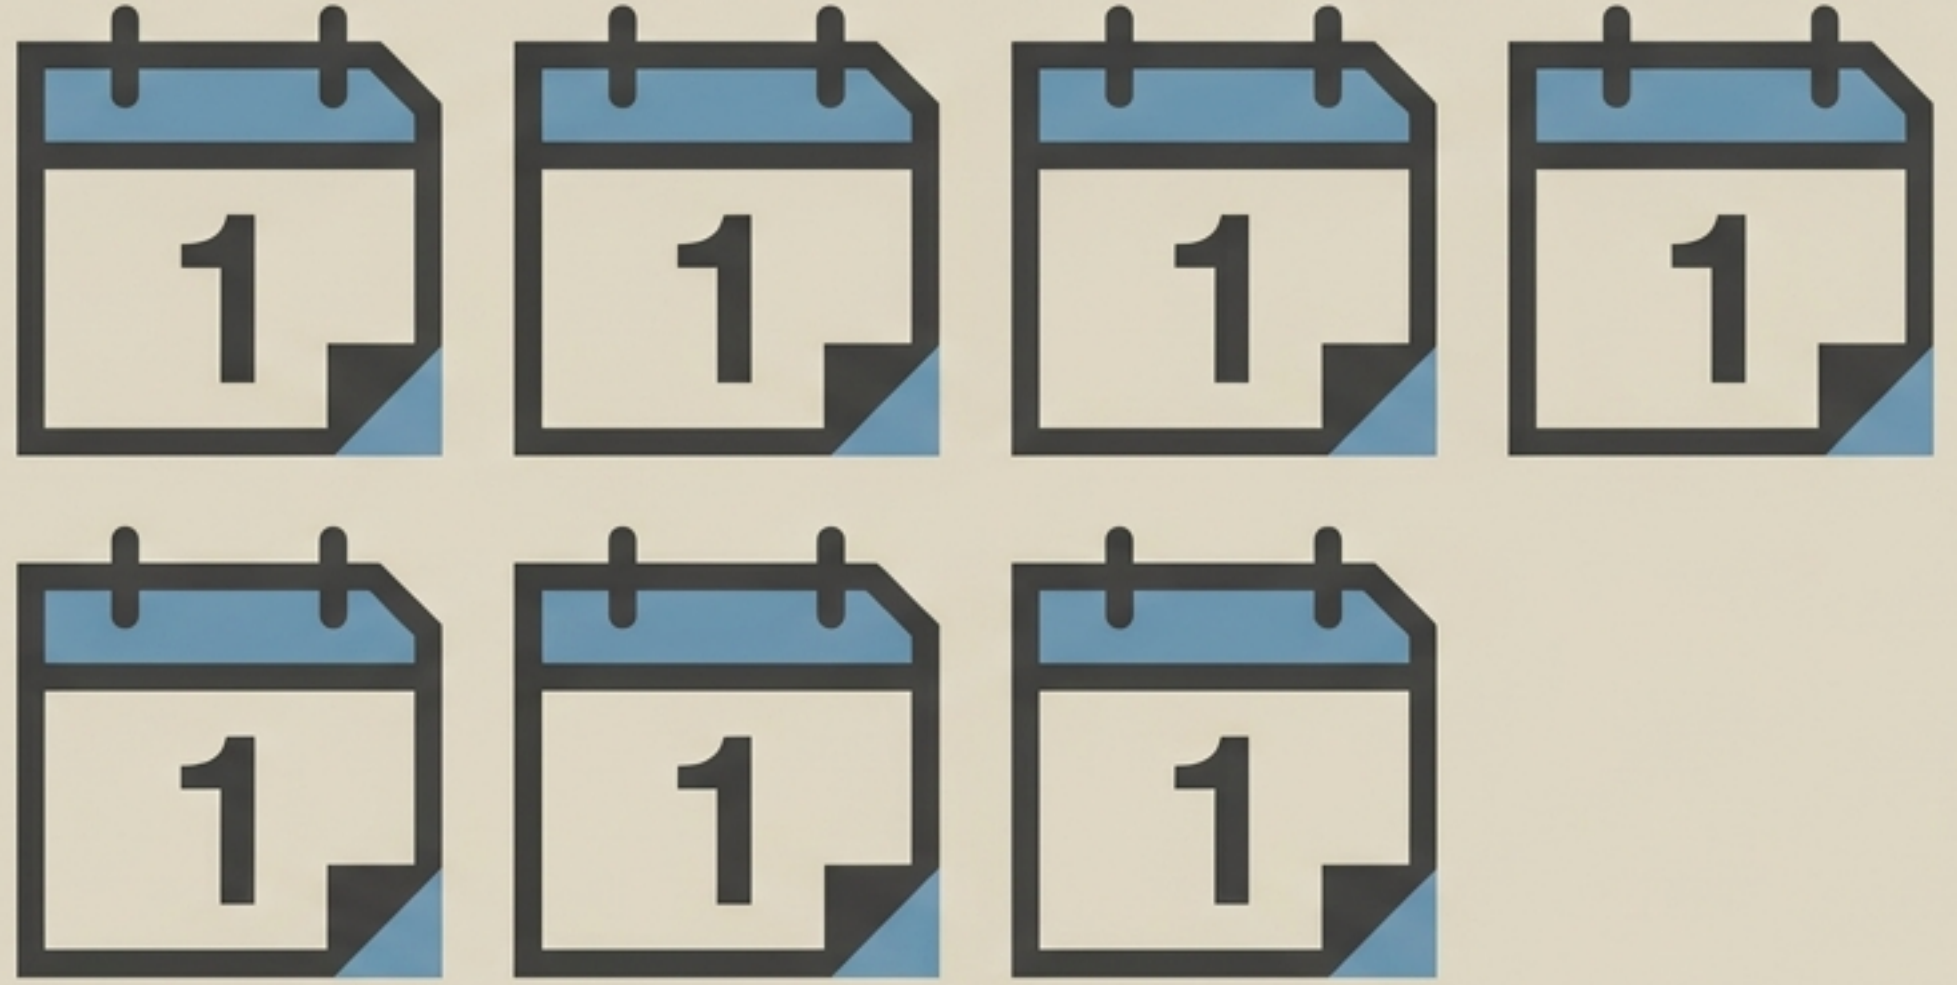

Every 7 days.

**Routine biological monitoring ensures the autoclave actively destroys all bacterial spores.
TEST AUTOCLAVES WEEKLY**