


FILL CARTRIDGE WITH INK

HOLD TIP UPRIGHT

OPERATE PLUNGER 50 TIMES

EN 17169 REQUIRES NO LEAKAGE

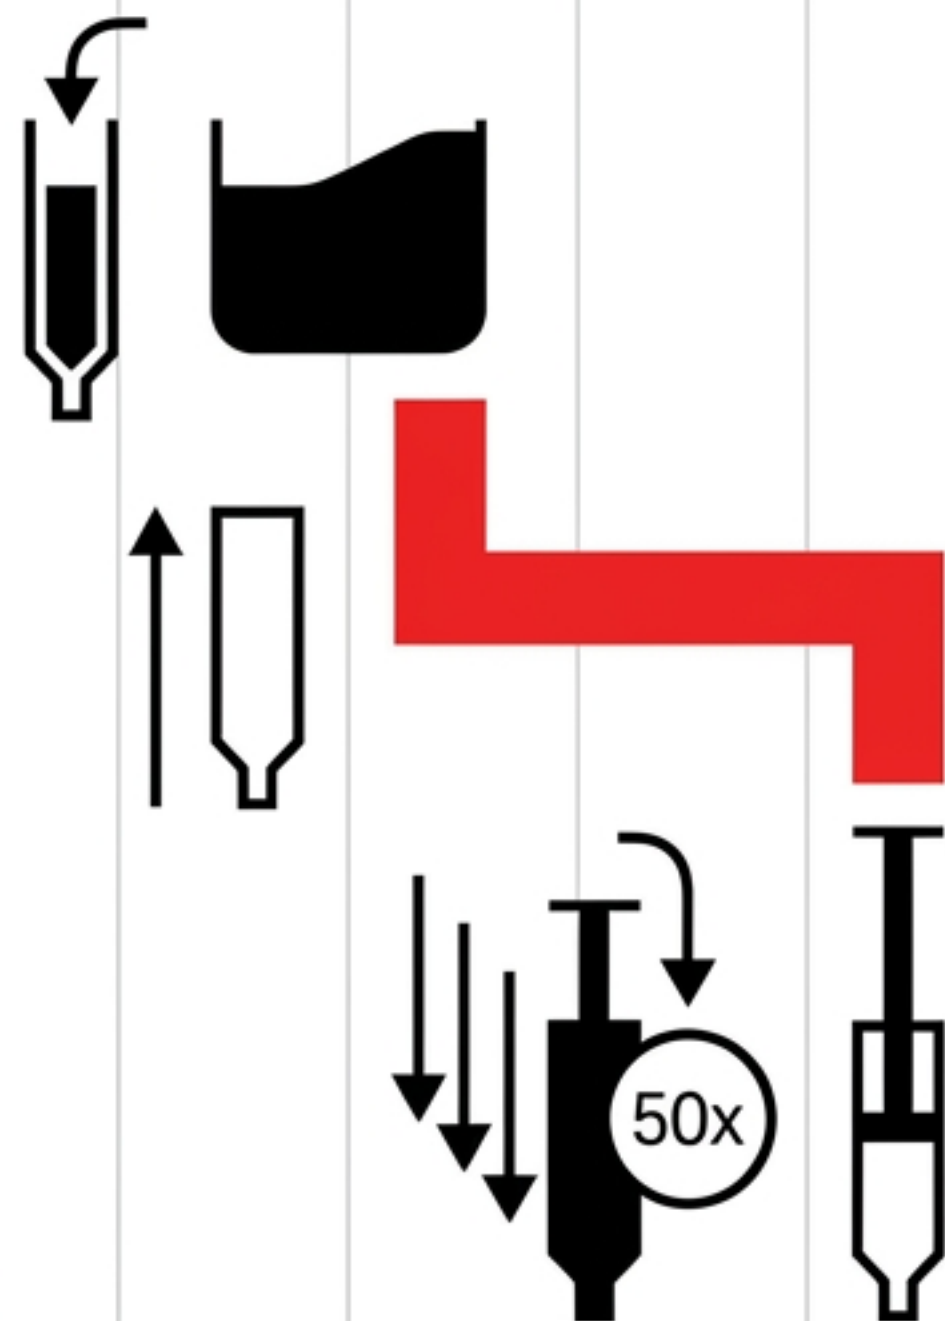

Testing confirms the membrane prevents body fluid ingress.

DOCUMENT PROOF OF SEALED CARTRIDGES.