


PLATE 1891

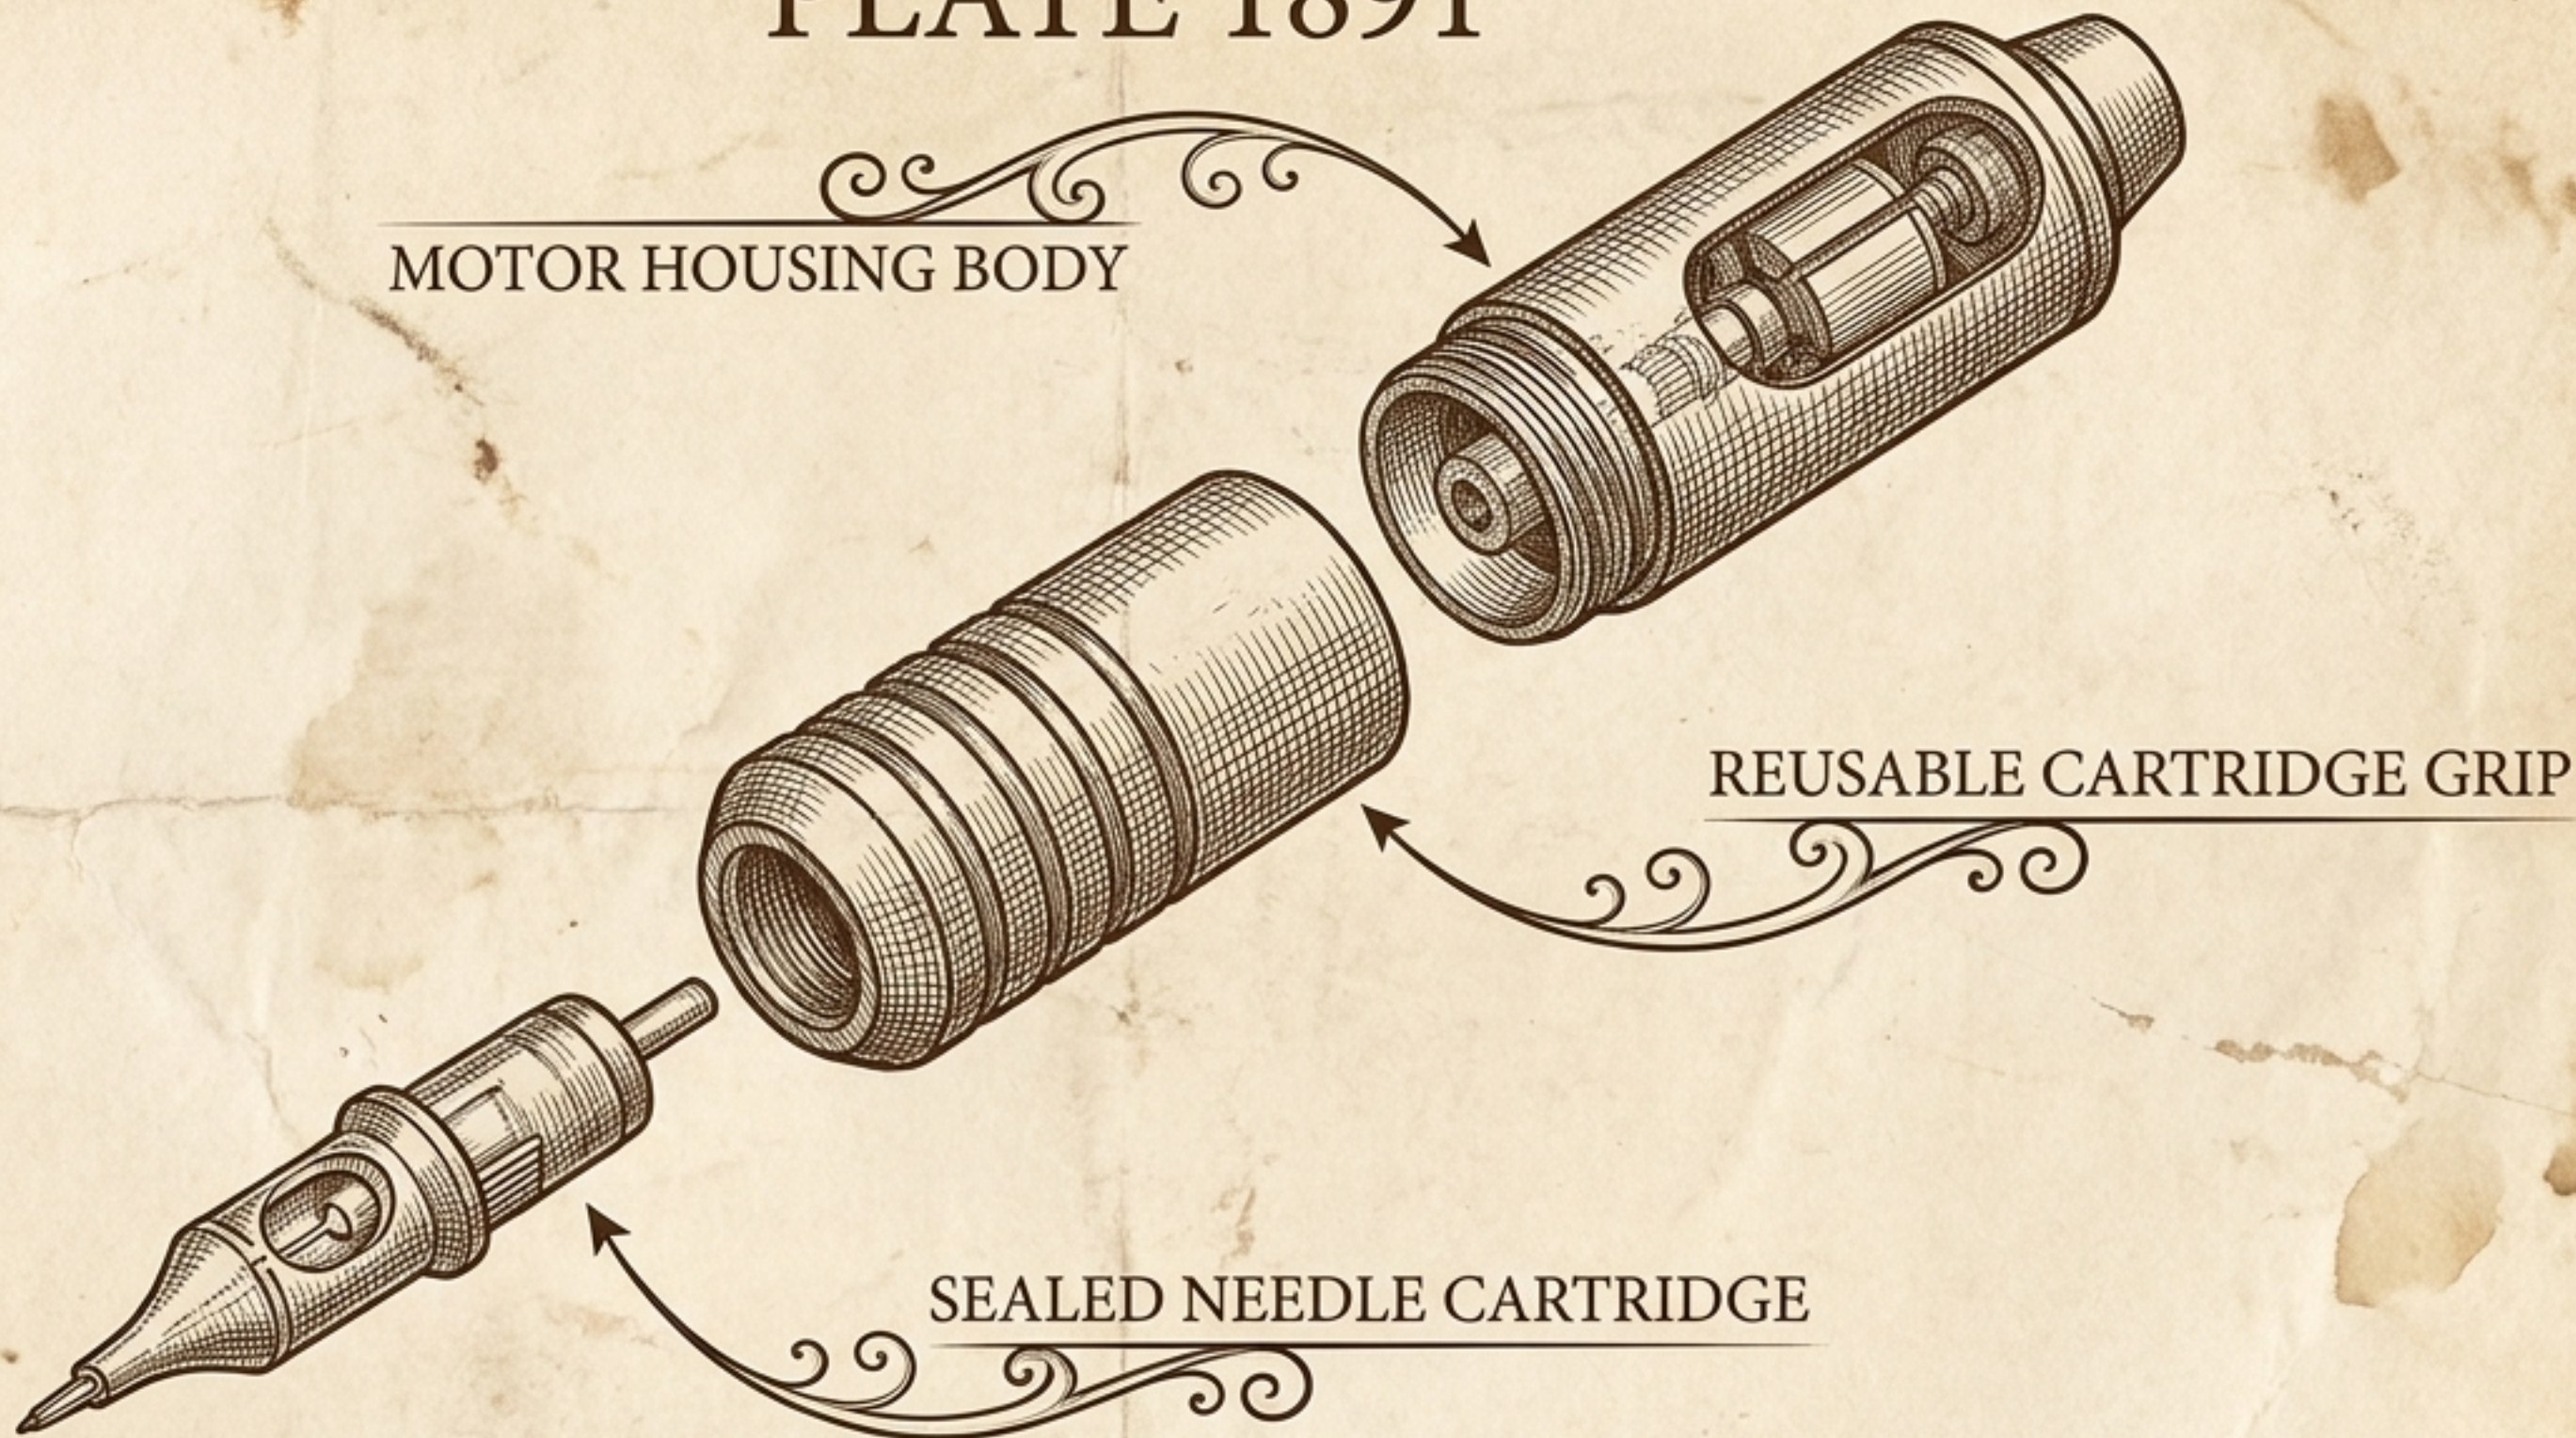

The membrane separates the contaminated needle from the clean grip.

DISCARD SINGLE USE CARTRIDGES IMMEDIATELY.