
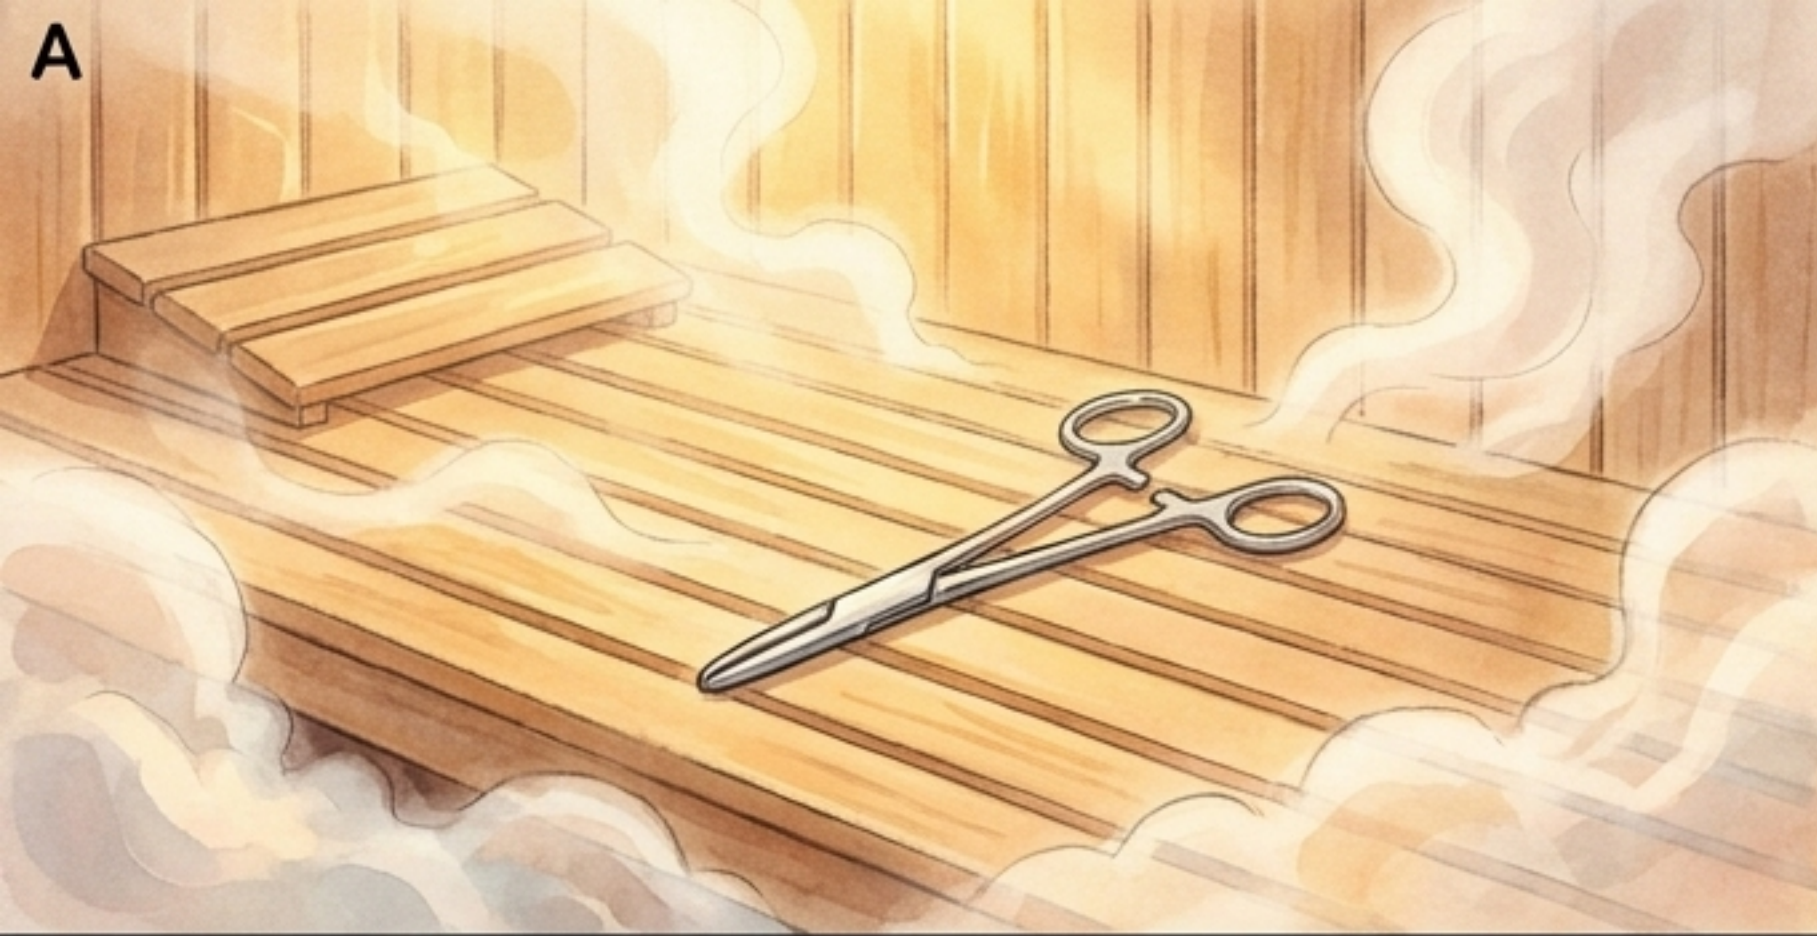


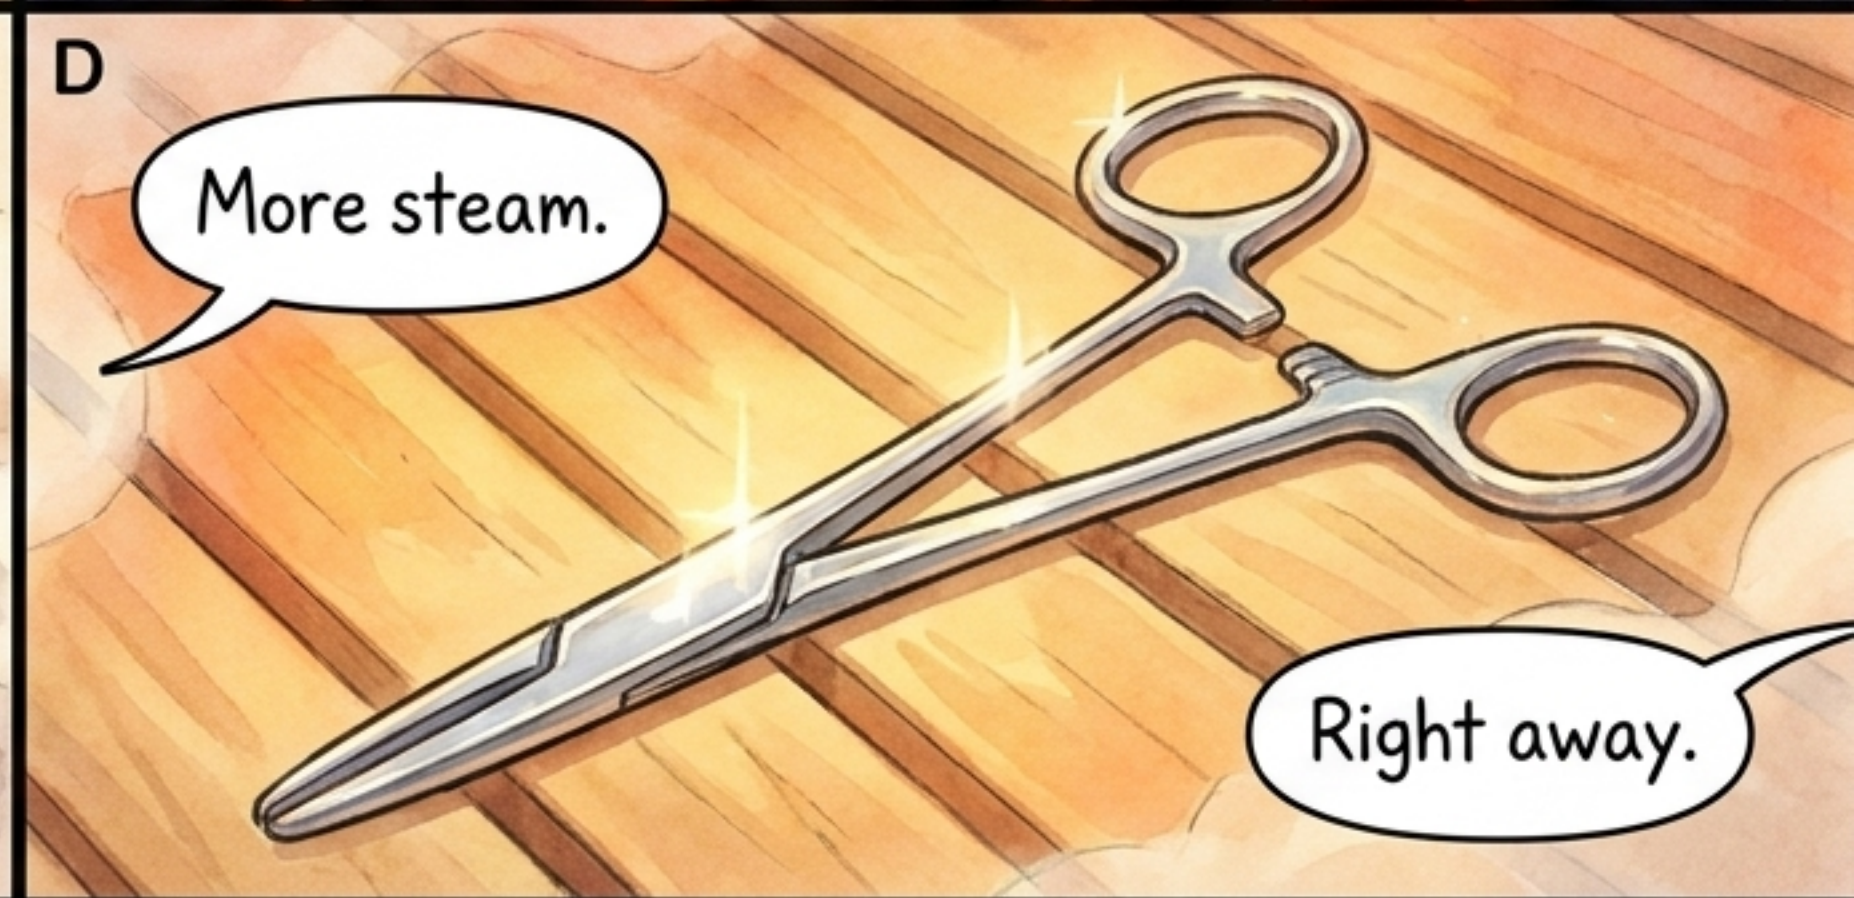

Reusable equipment must undergo intensive autoclave sterilization combined with regular biological spore testing.
Spa day for the clamps.