



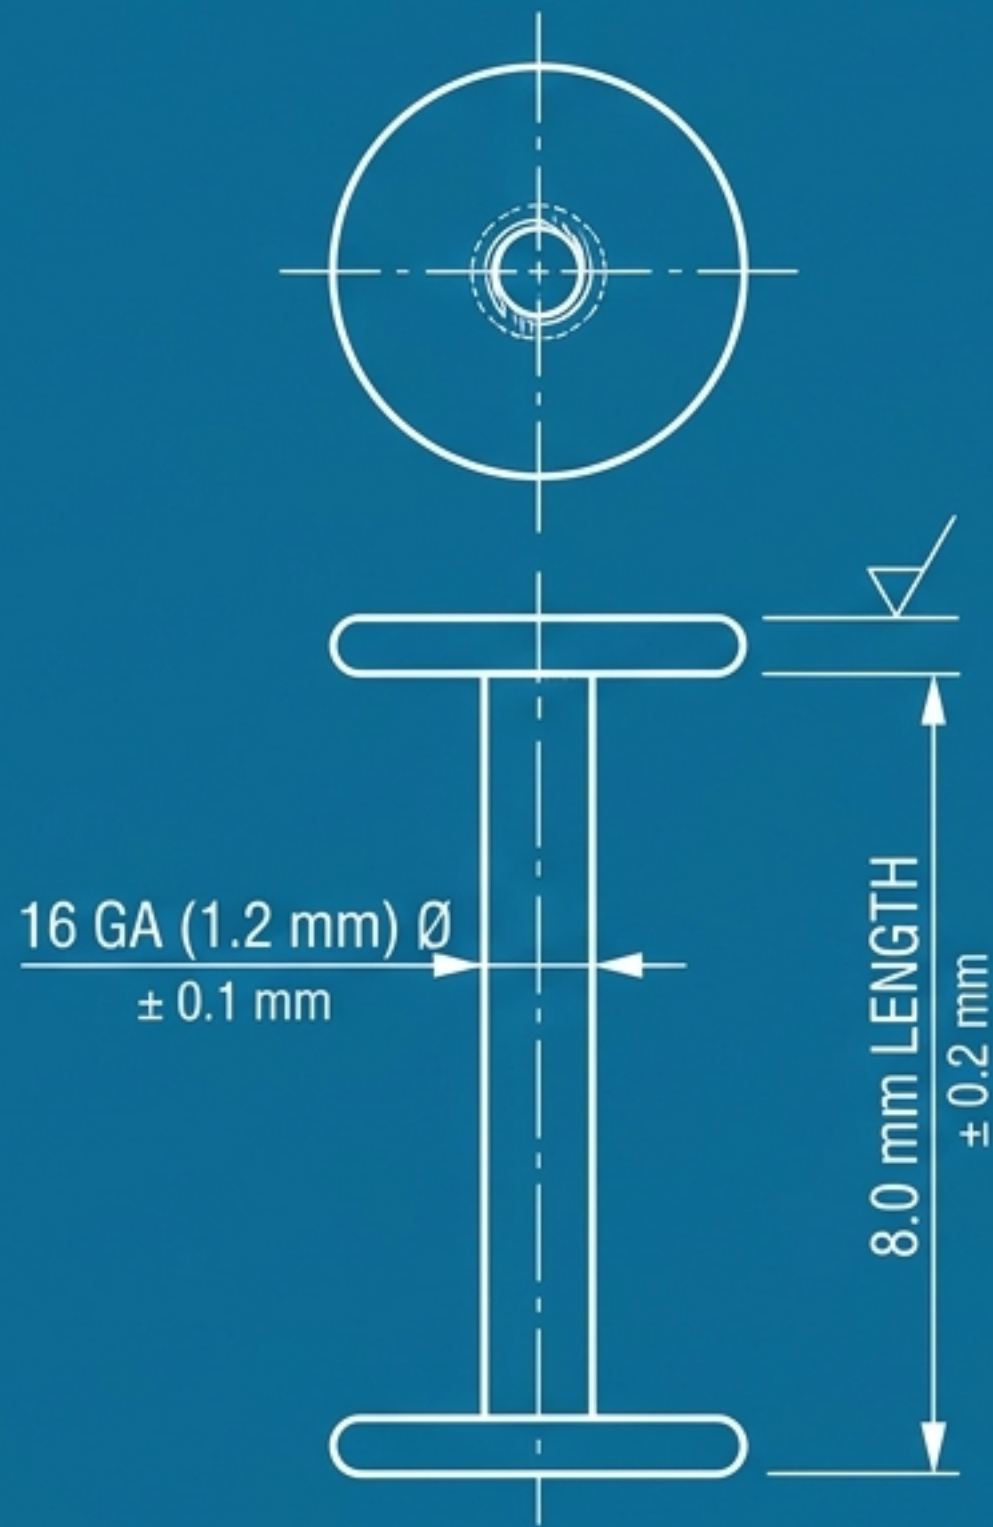

Lobe takes
16 gauge studs.

Shaft length
measures
8 millimetres.

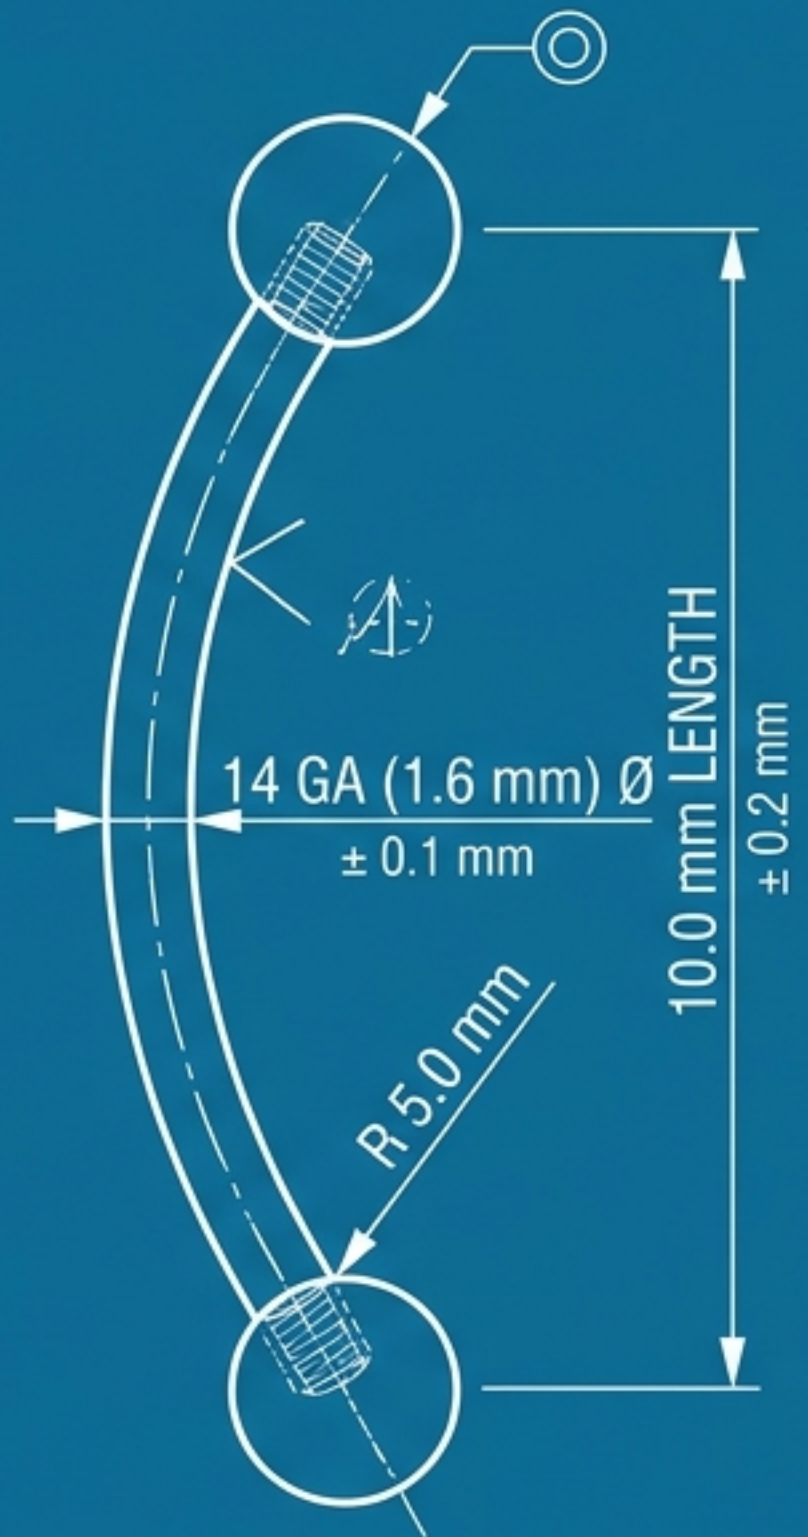

Navel takes
14 gauge
barbells.

Shaft length
measures
10 millimetres.

Implant titanium prevents dangerous nickel sensitization.
DEMAND MILL CERTIFICATES.