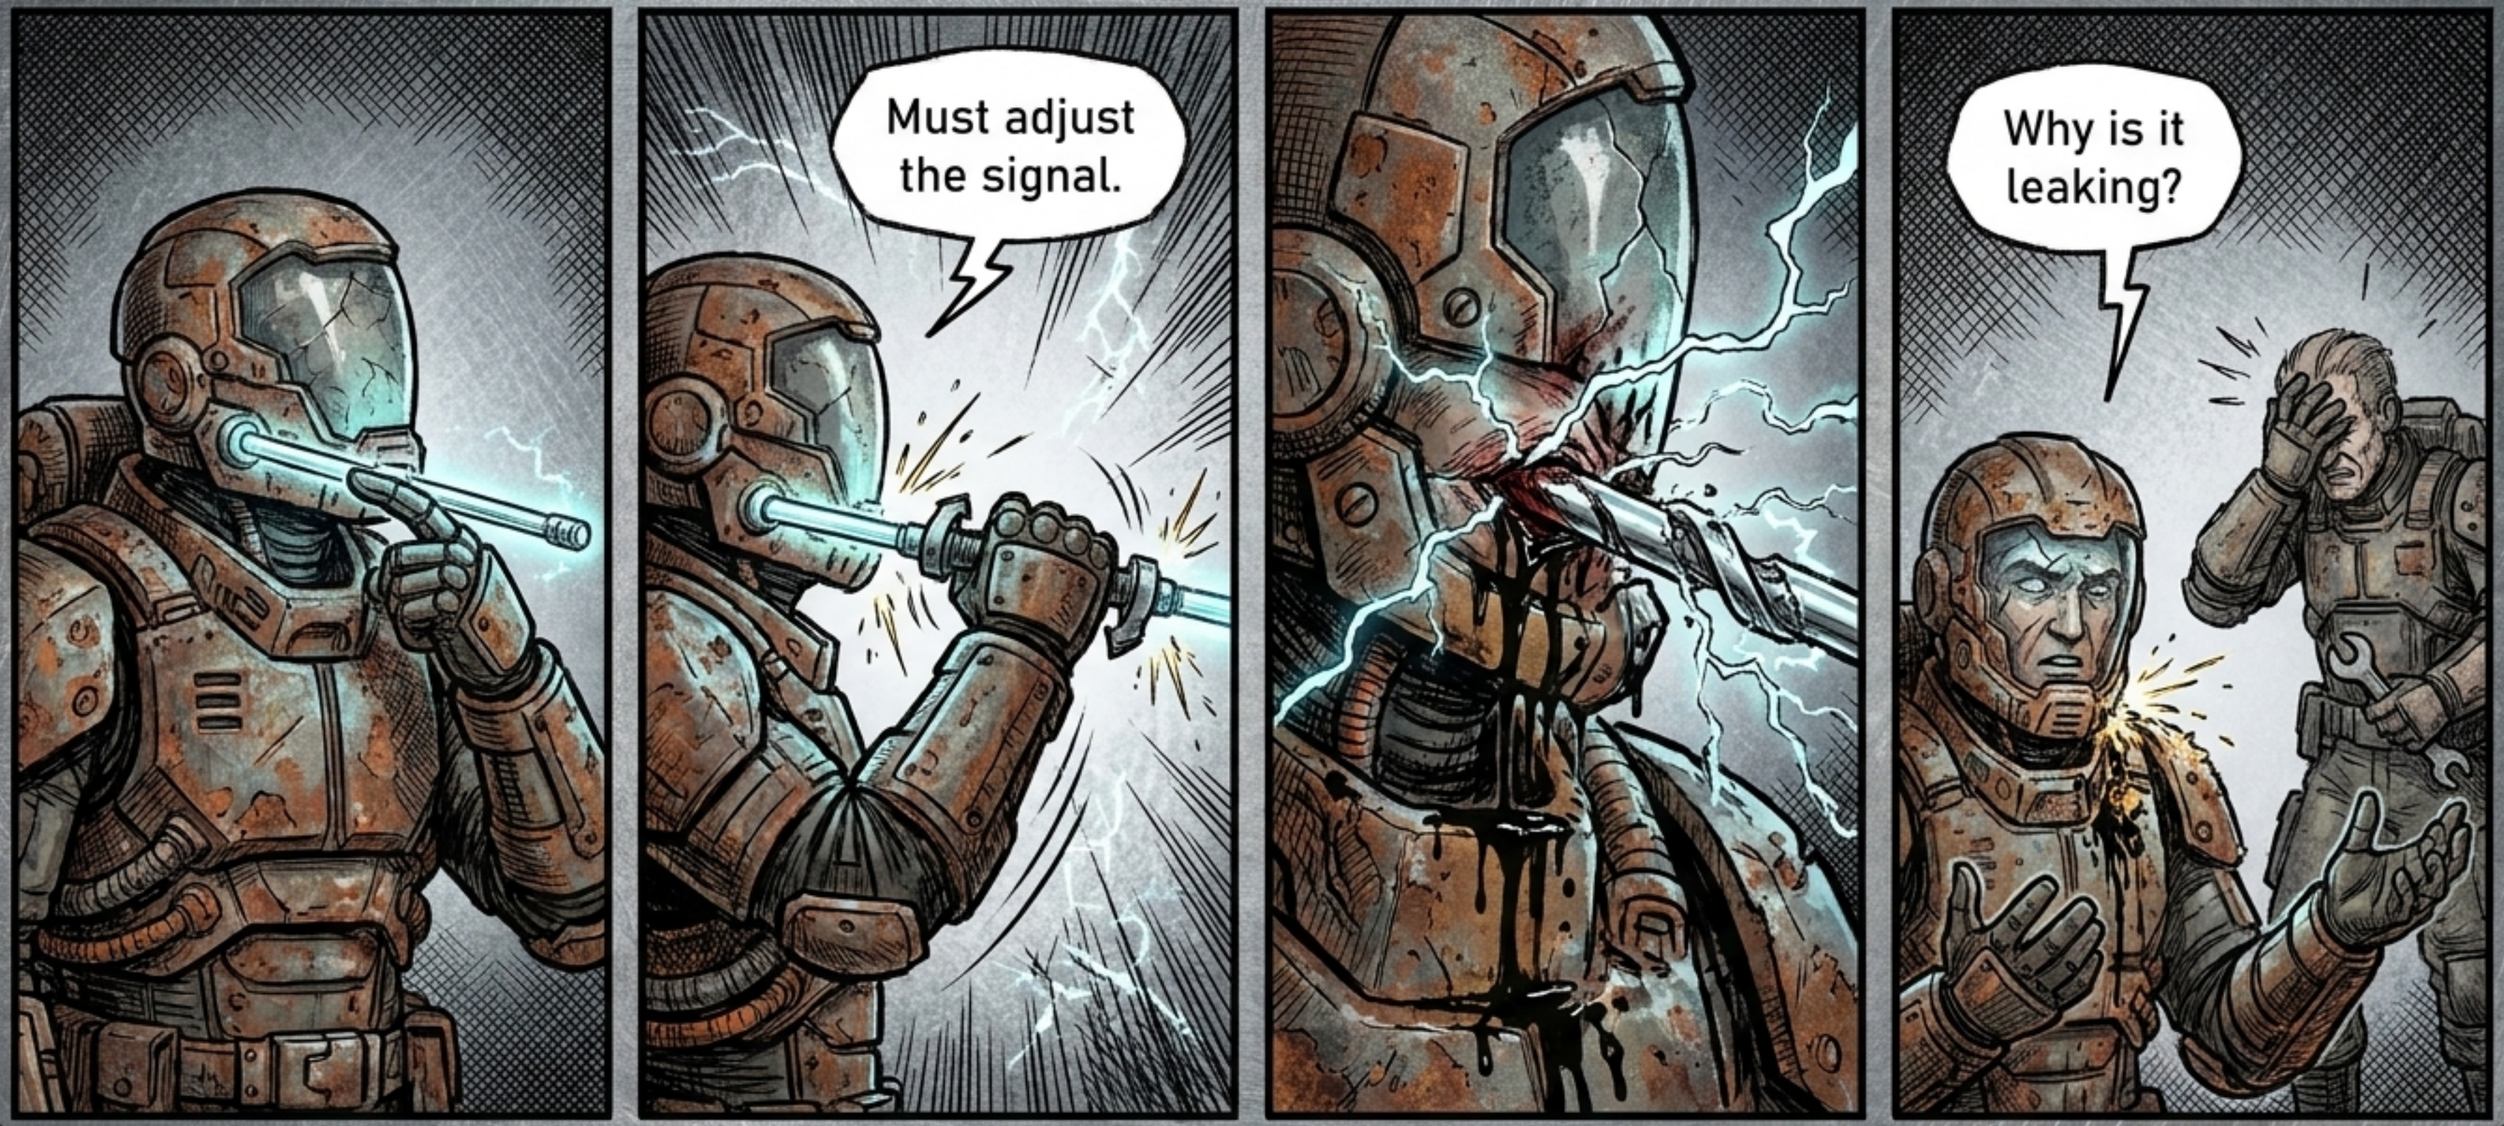

Rotating fresh jewellery tears the delicate cellular seal and reopens the healing channel to contamination.
Treating a fresh implant like a radio dial guarantees terrible reception.