


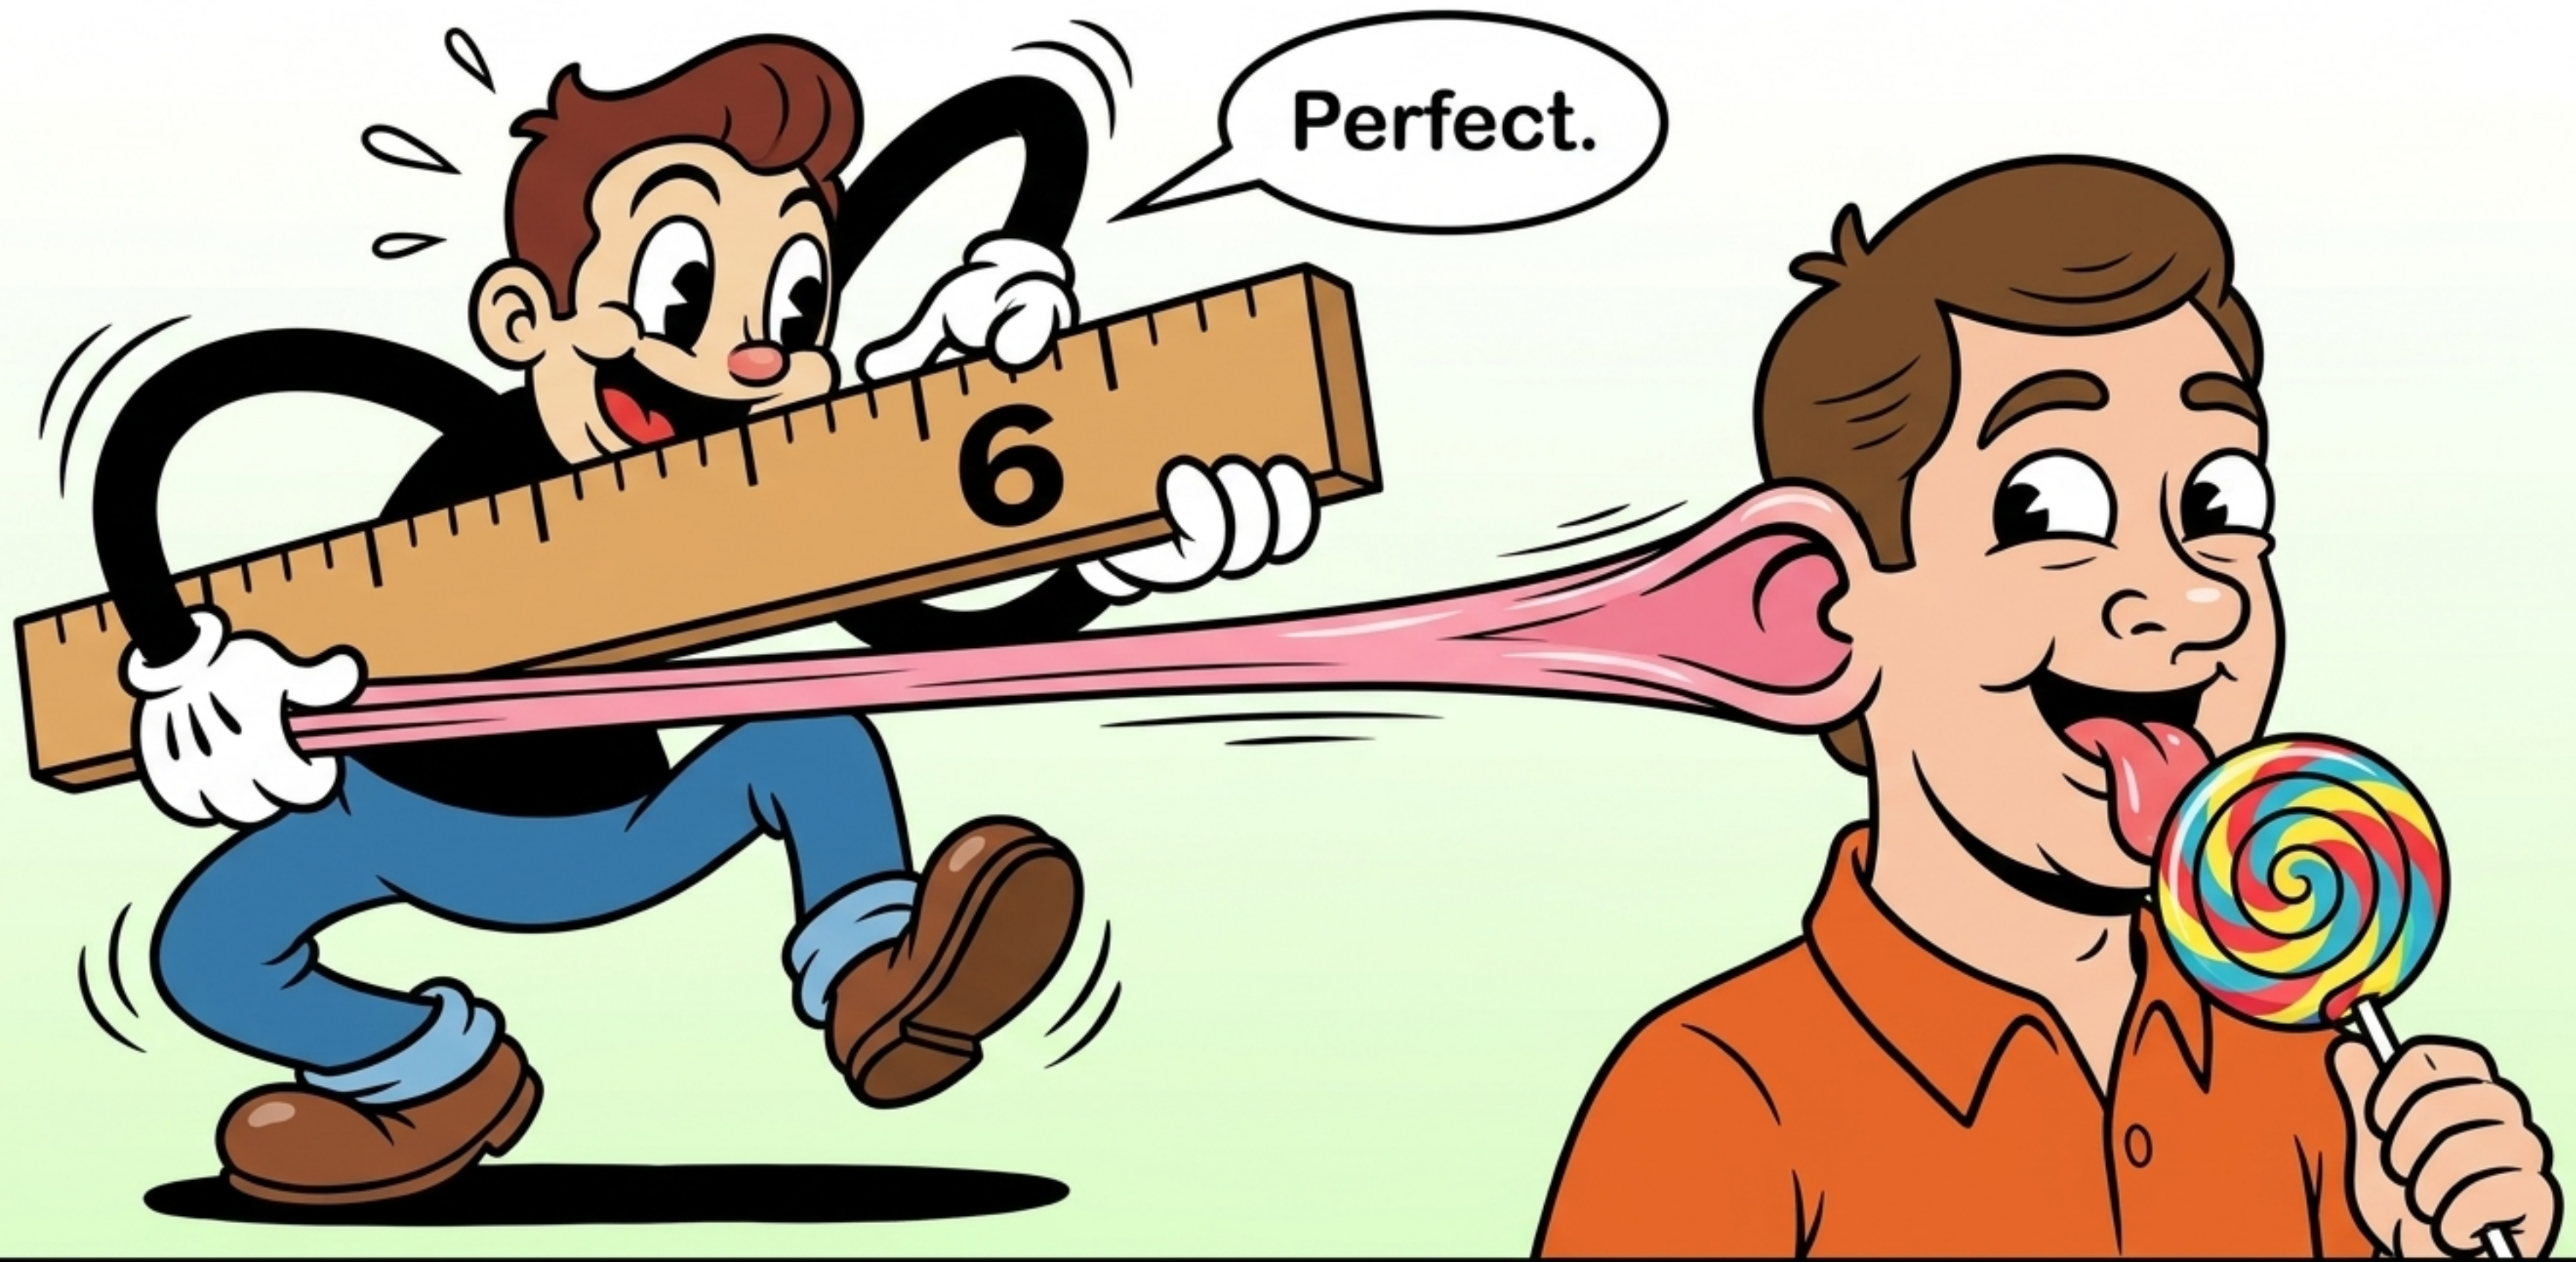

Six millimetres of tissue depth is the minimum for piercing stability.

Bending the fabric of reality beats calibrating the instruments.