
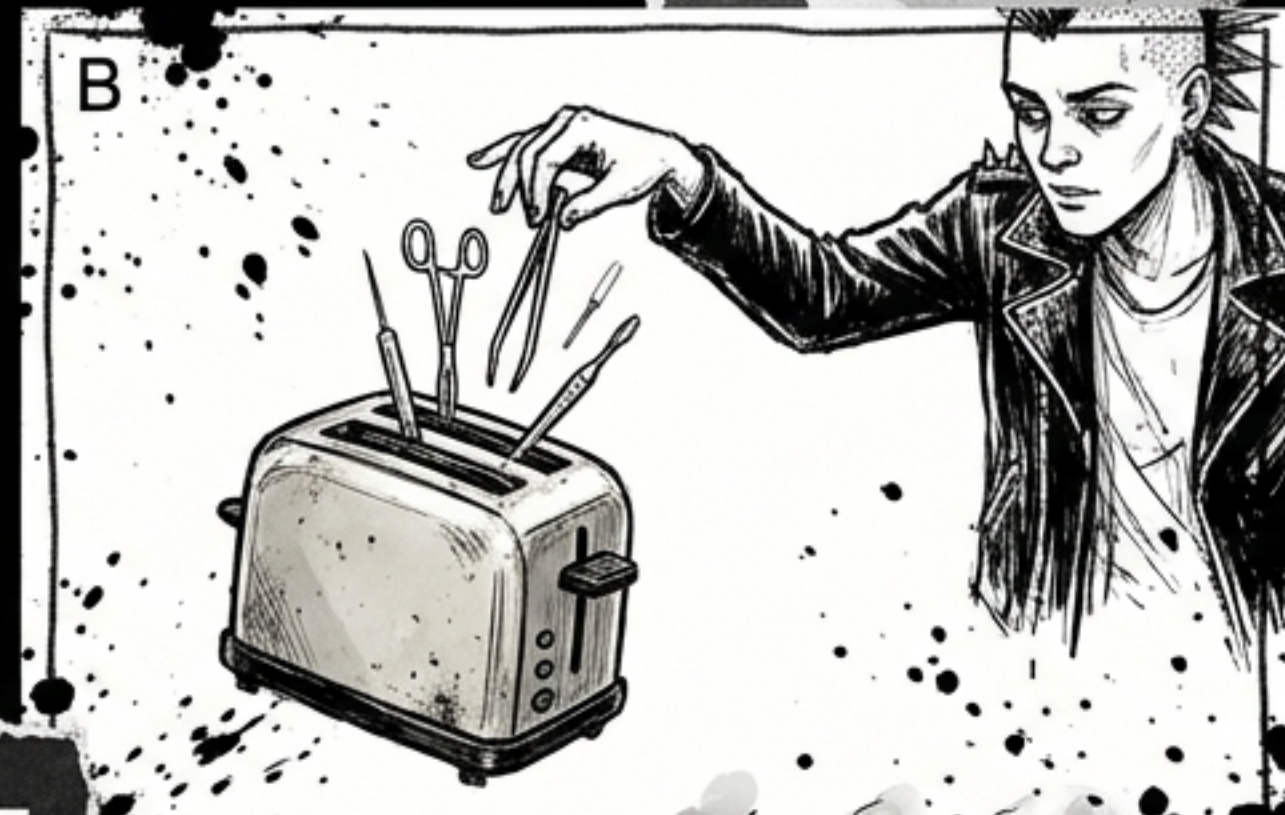


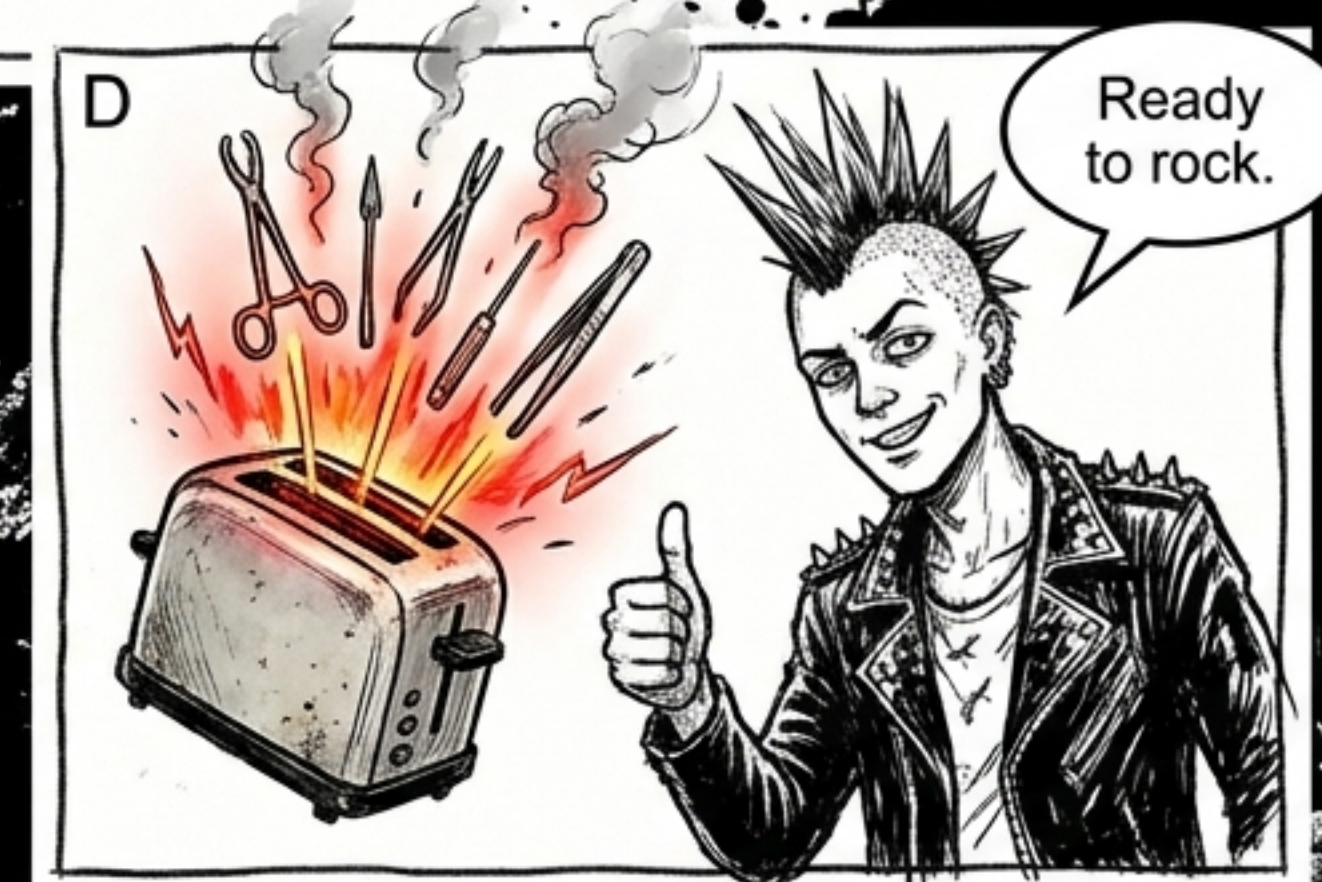

Reusable equipment must undergo autoclave sterilization using extreme heat and pressure to eradicate pathogens. Household toasters lack the necessary clinical authority.