


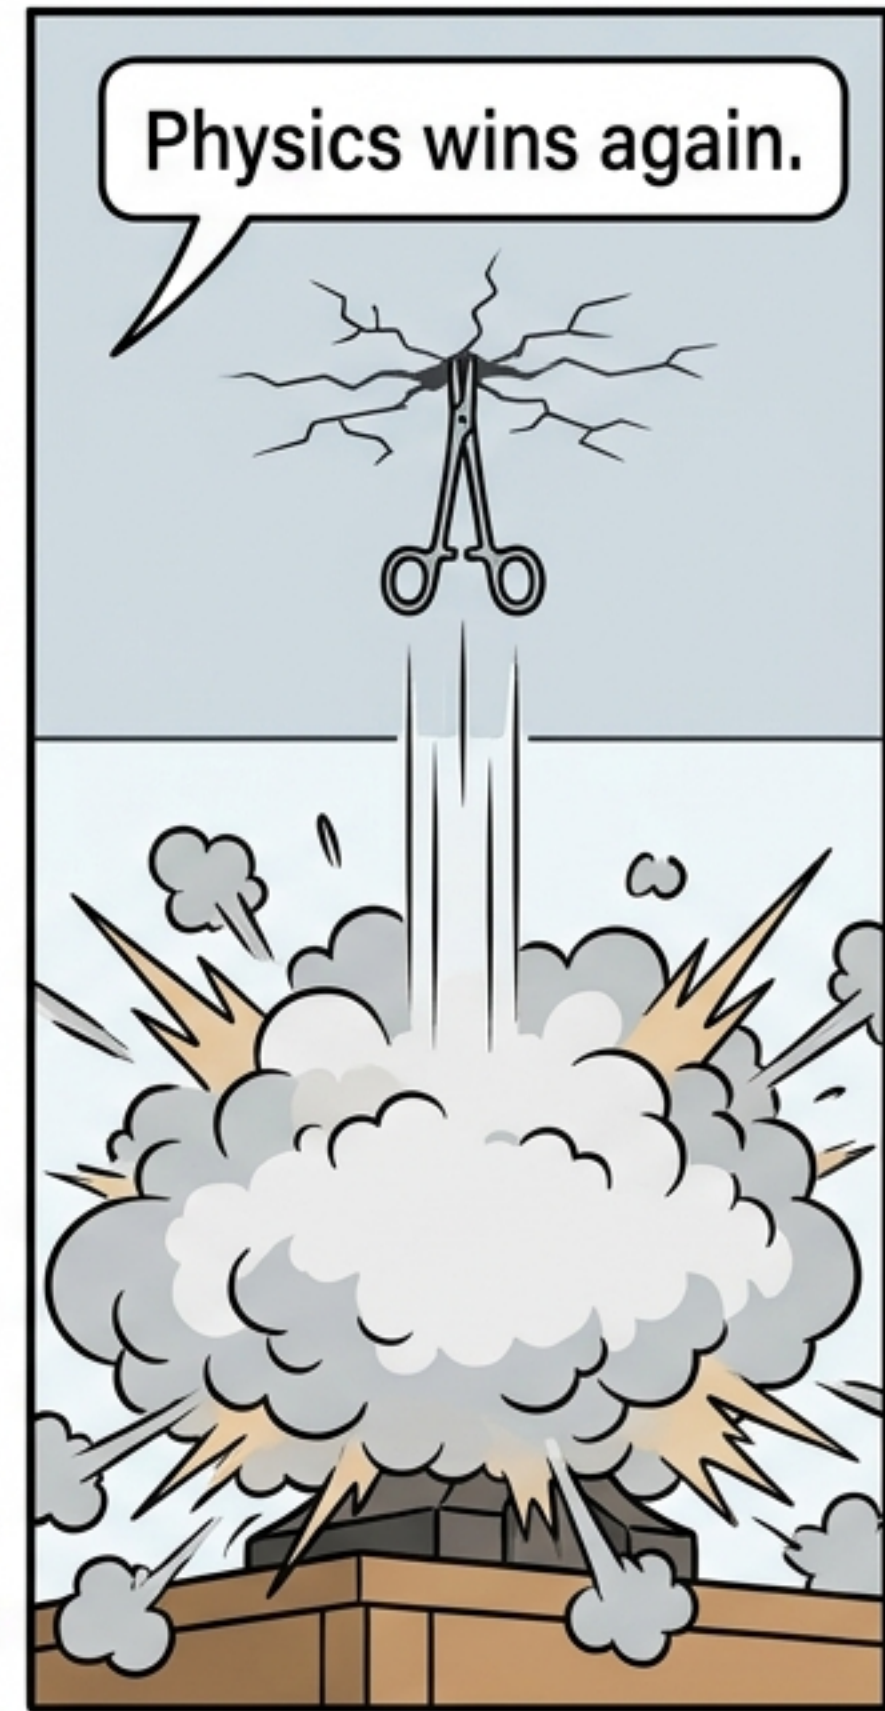

Gravity displacement sterilizers rely on passive thermodynamic exchange and cannot reliably purge air from sealed sterilization pouches.

The laws of physics politely decline to open paper bags.