


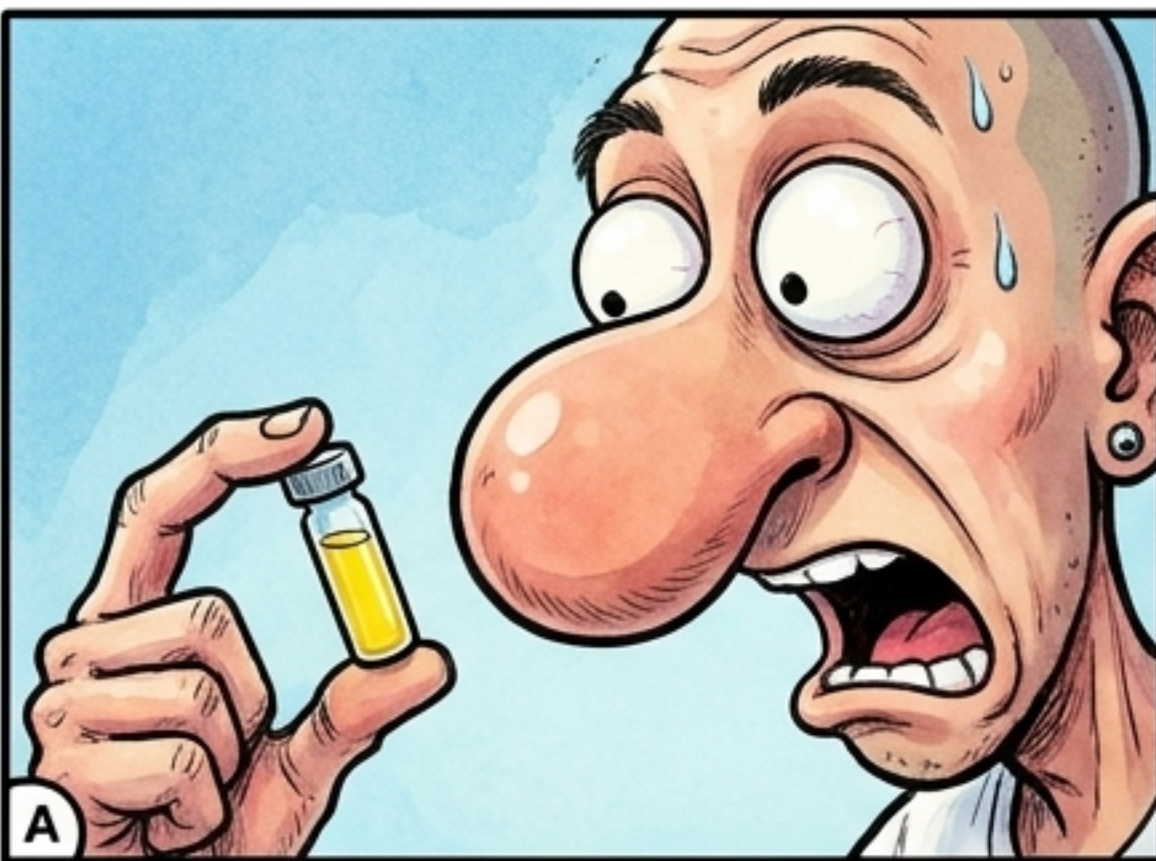

All instruments processed within the exposure window must be moved to a clearly labelled quarantine area.
Building a fortress of warning tape around the instrument cabinet is a perfectly rational response to a positive spore test.