


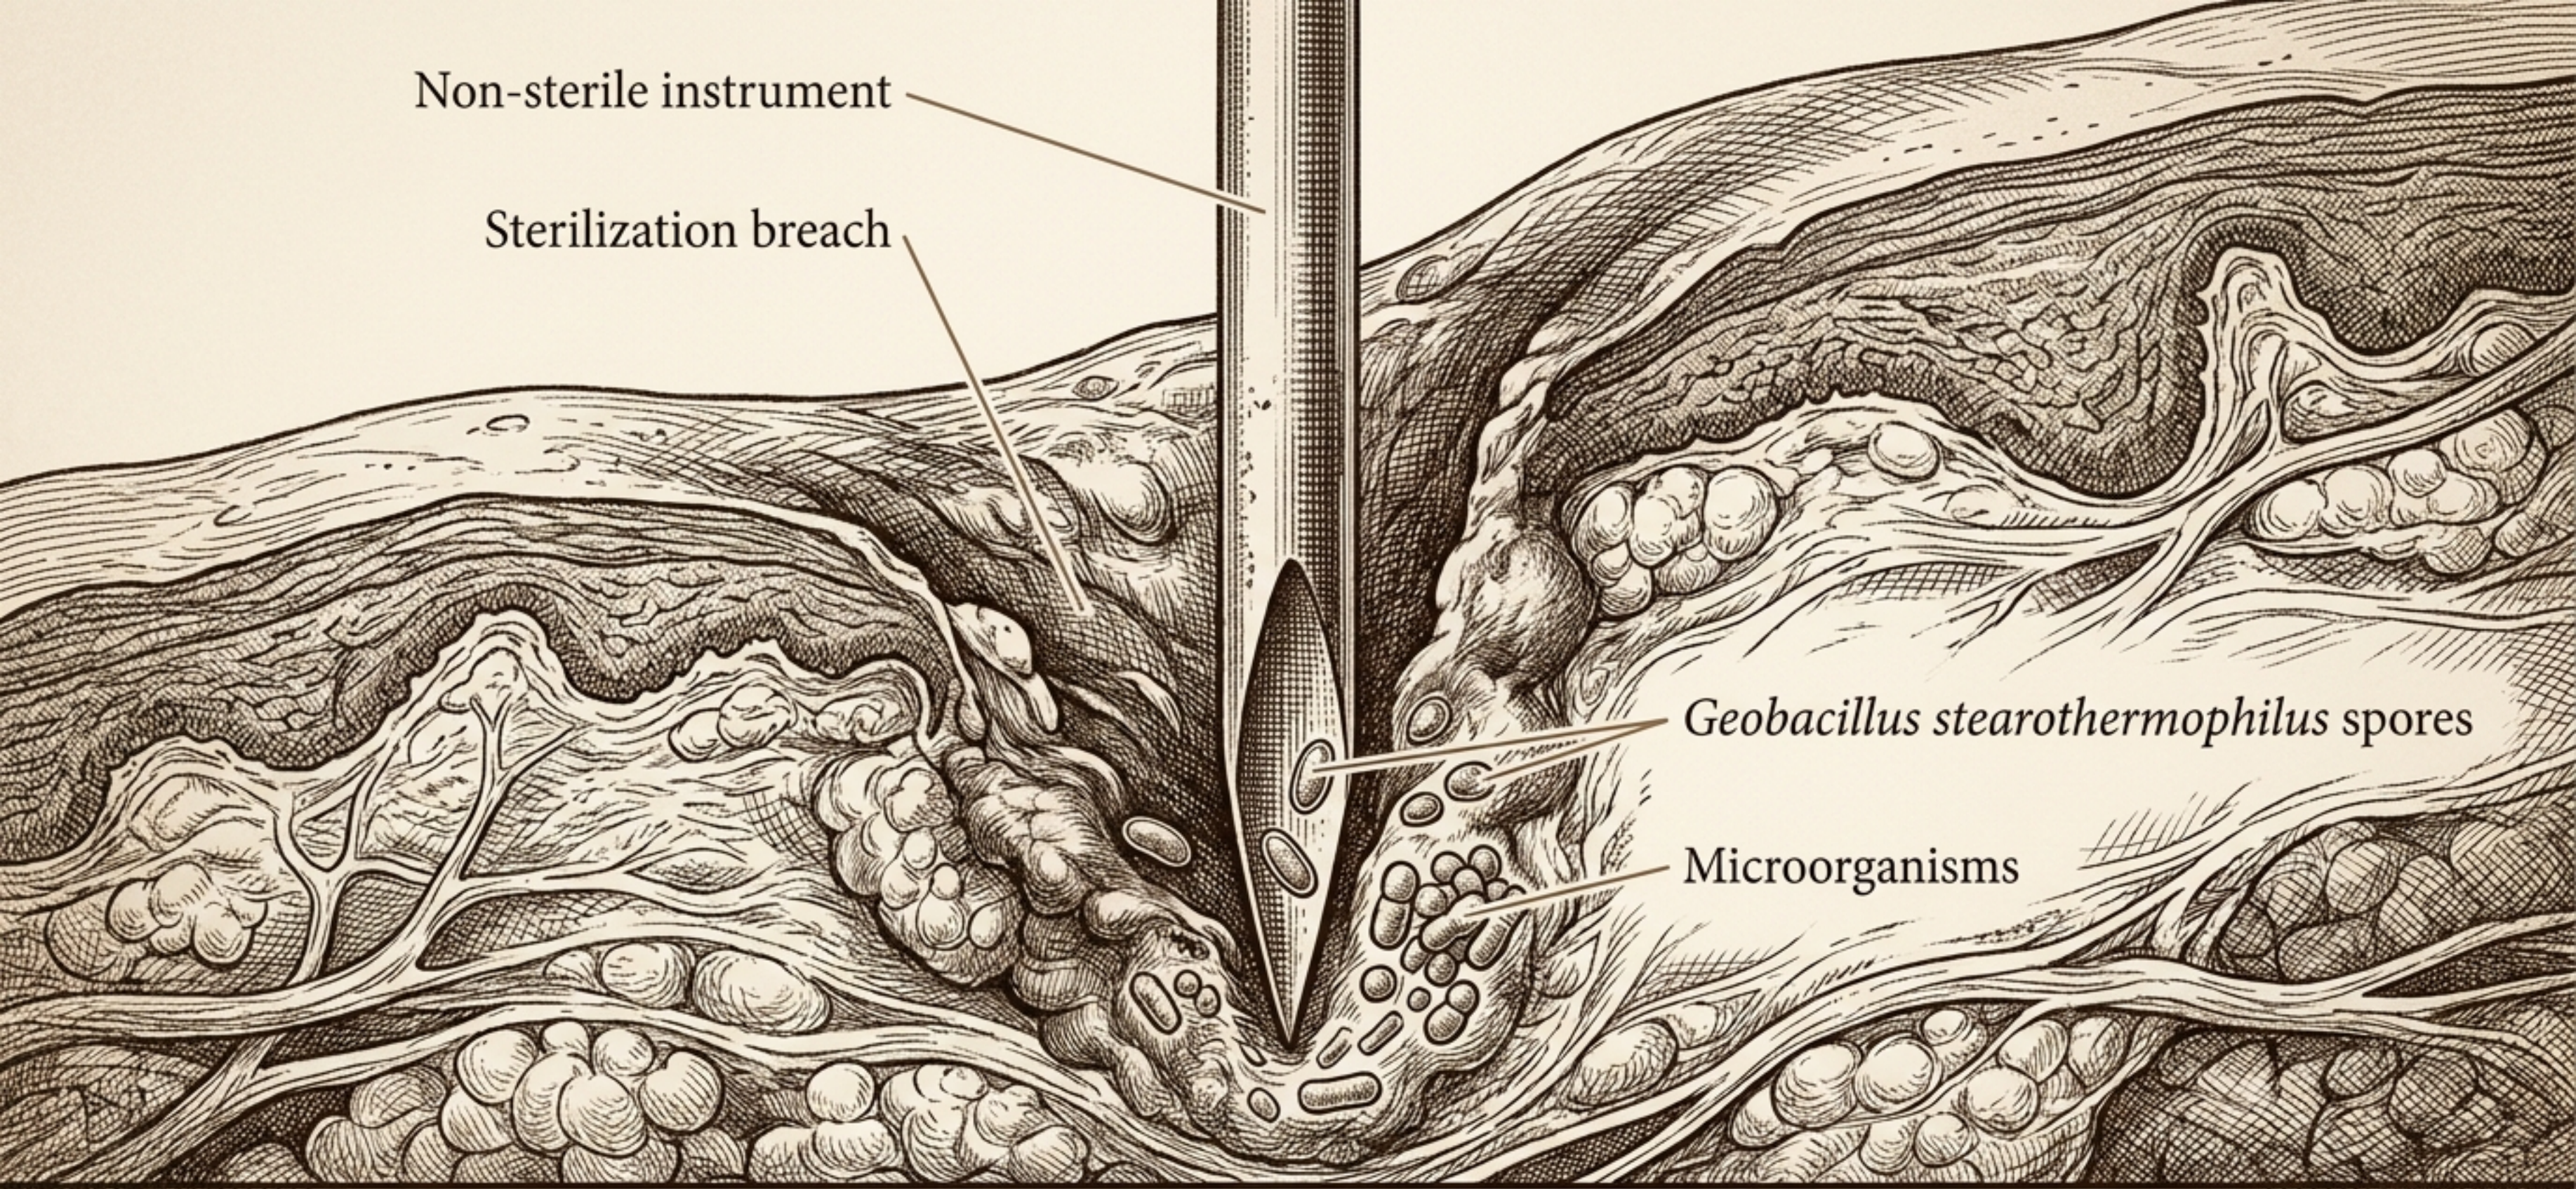

Non-sterile instrument

Sterilization breach

Geobacillus stearothermophilus spores

Microorganisms

A positive spore test is a confirmed sterilization breach.

TREAT EVERY FAILURE AS CONFIRMED.