


Surviving spores
change medium color.

Yellow liquid
confirms a failure.

Purple liquid confirms
lethal conditions.

Control vial must
remain viable.

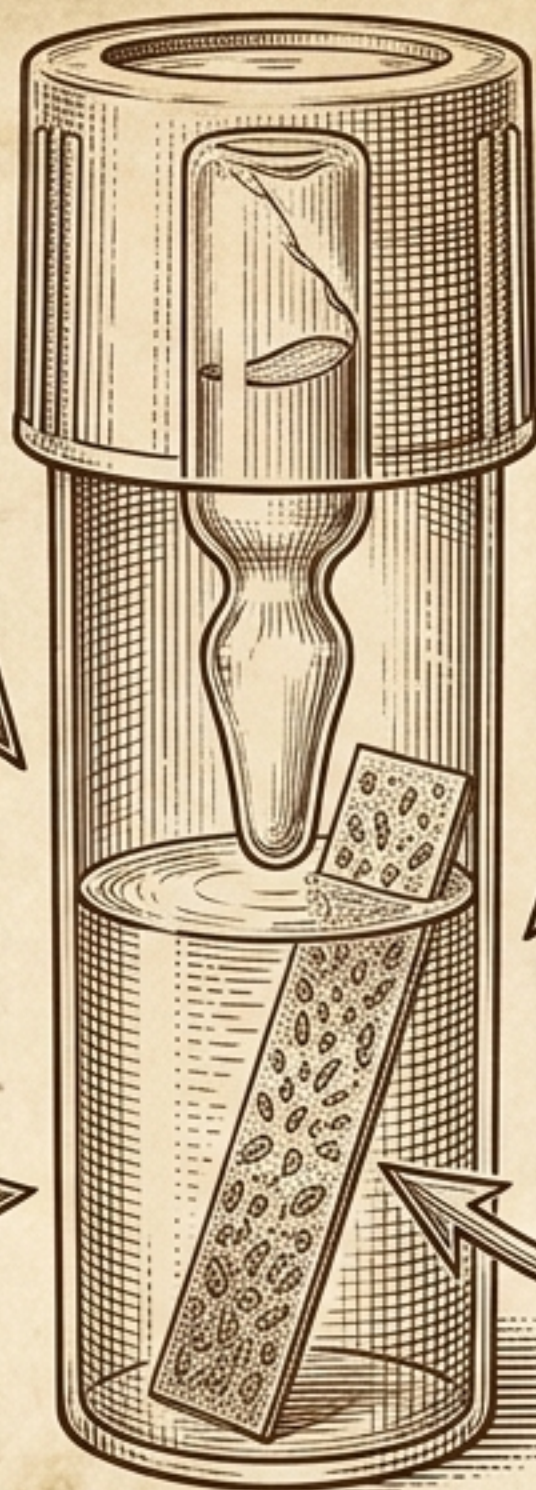

1

Chemical indicators only confirm steam presence rather than lethal conditions for spores.
ONLY BIOLOGICAL INDICATORS CONFIRM LETHALITY