


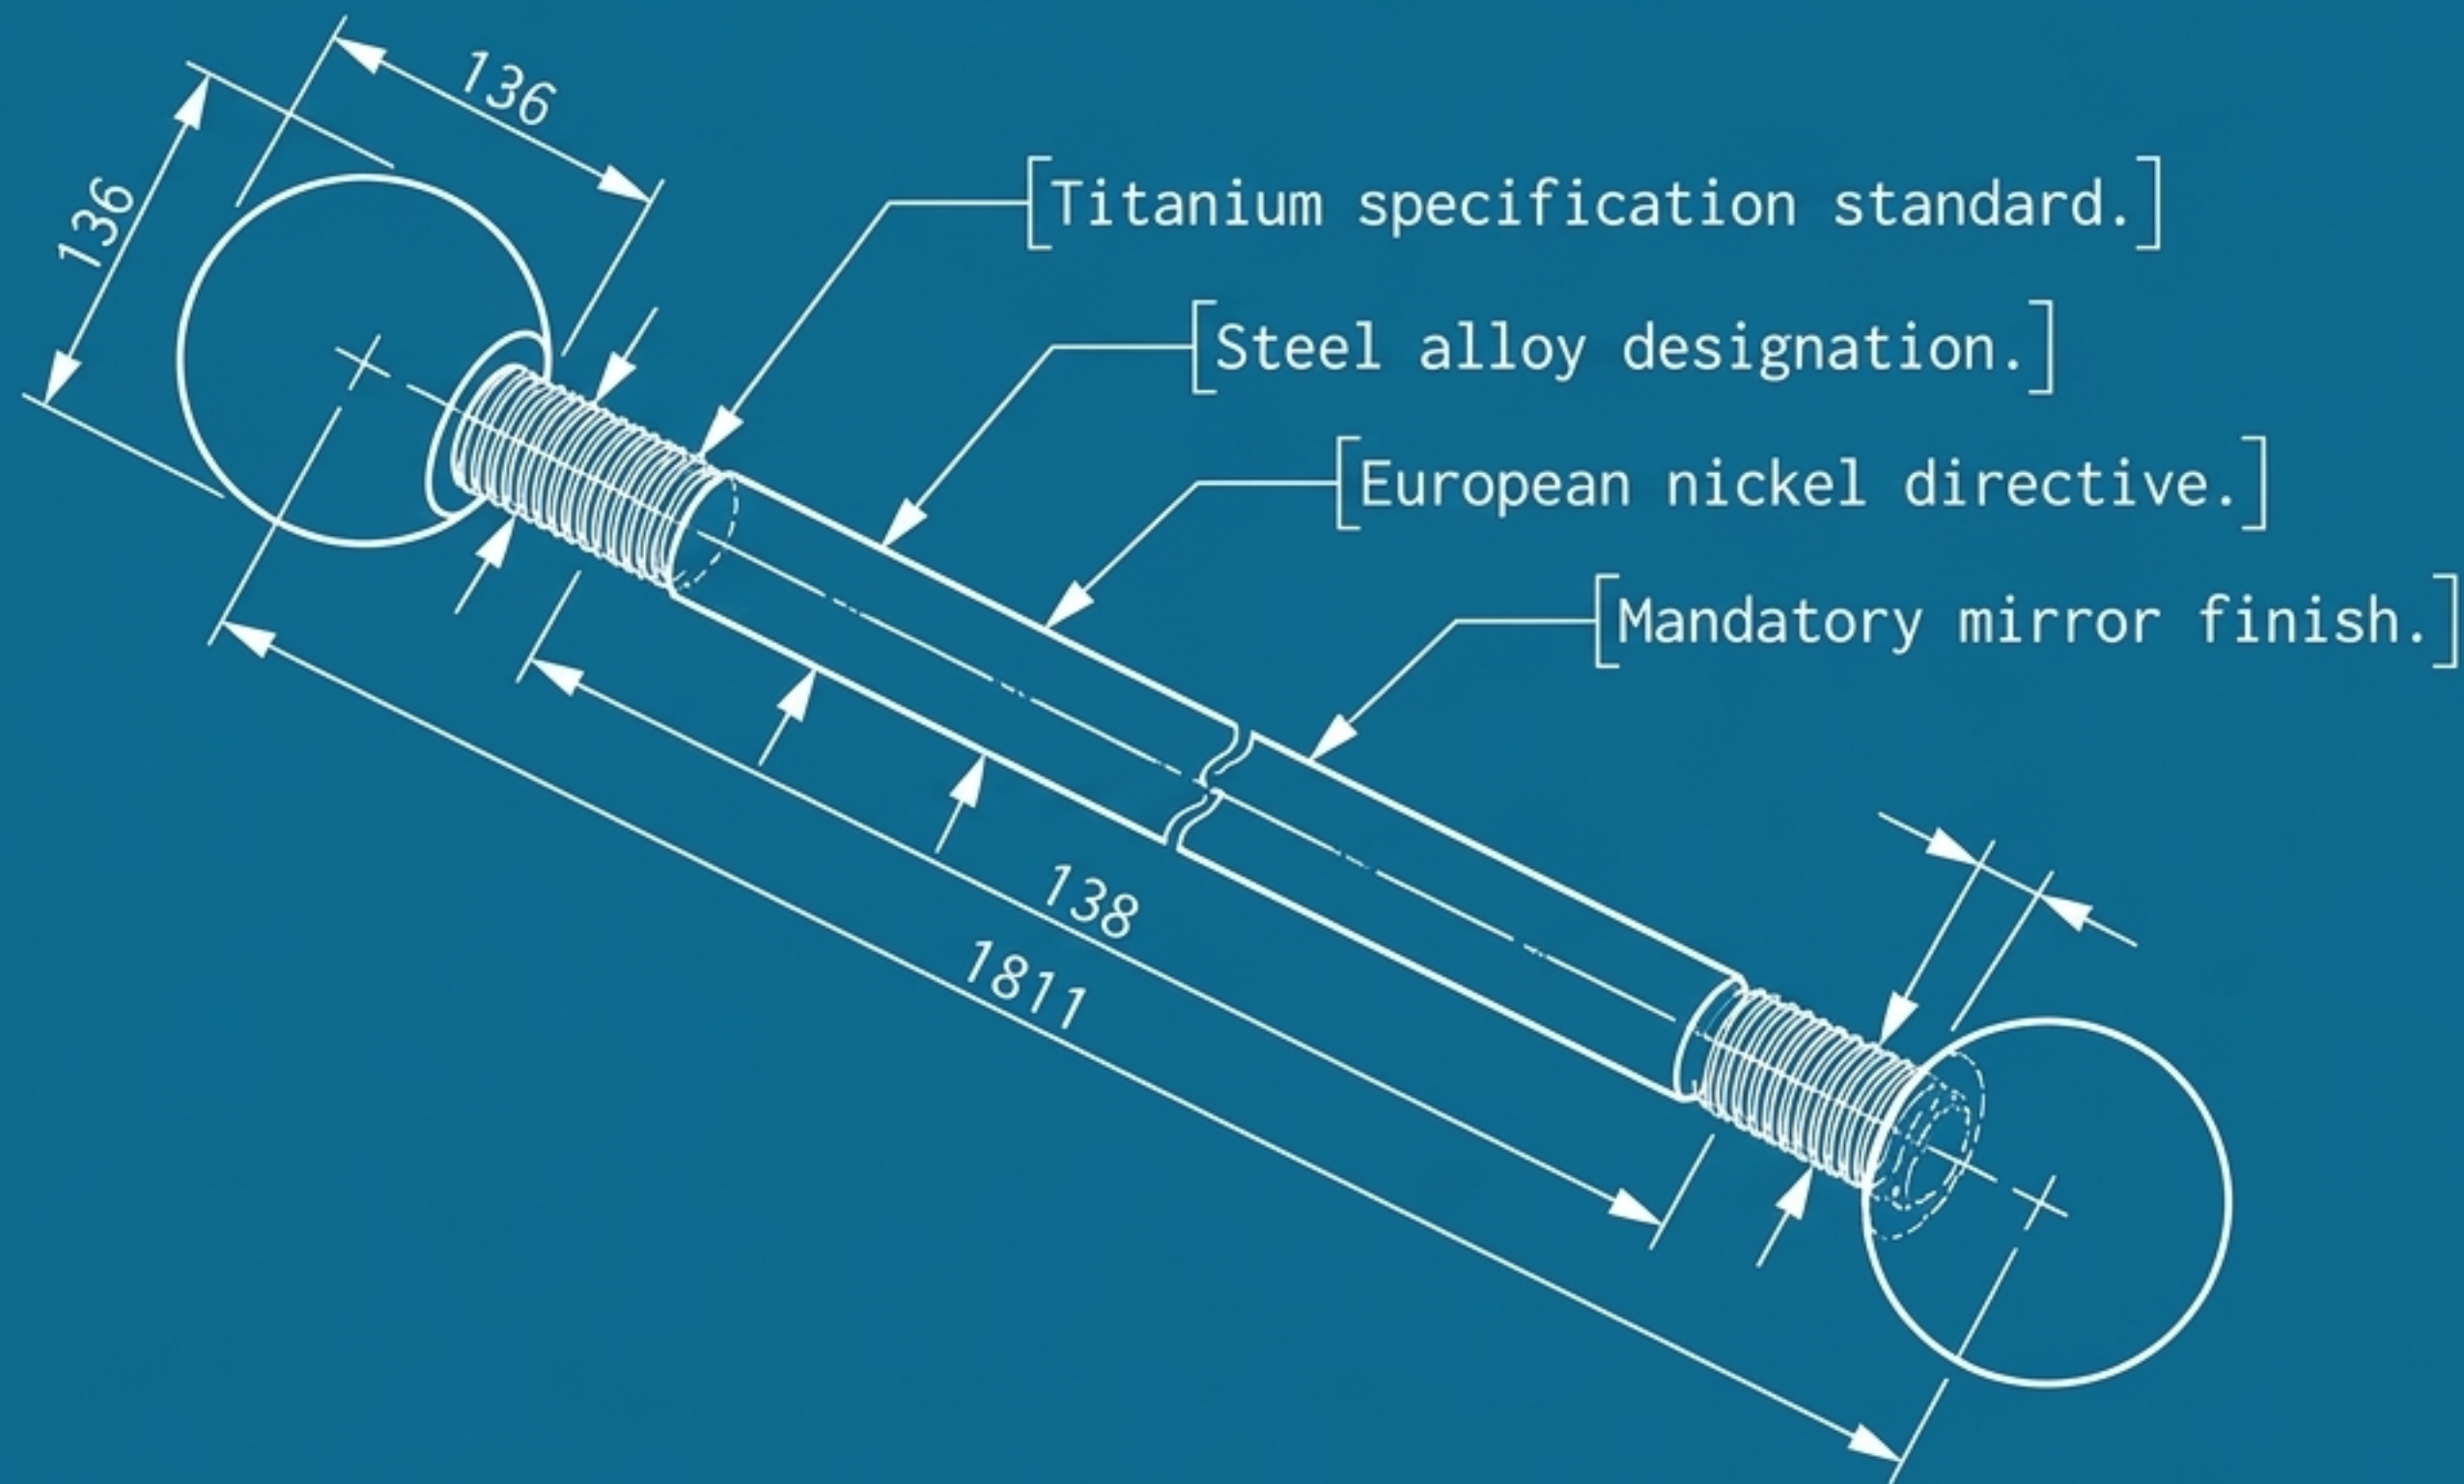

Implant-grade alloys require strict manufacturing specifications and documented biocompatibility.

Always verify mill certificates before initial piercing insertion.