
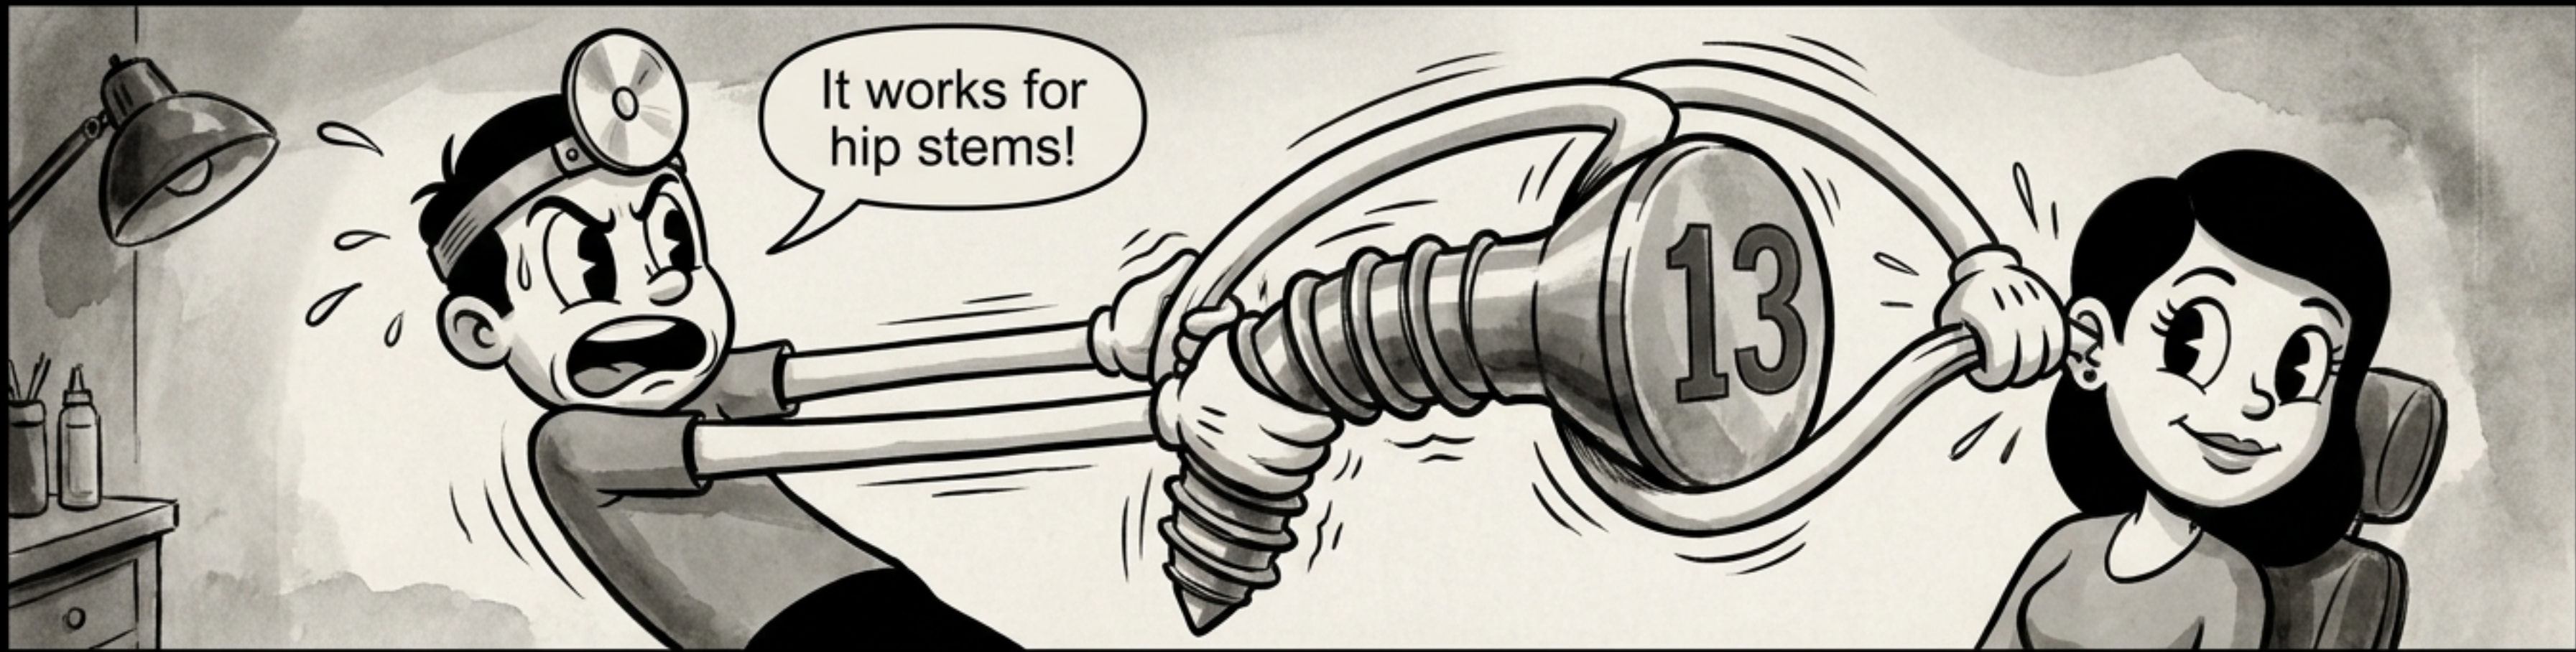


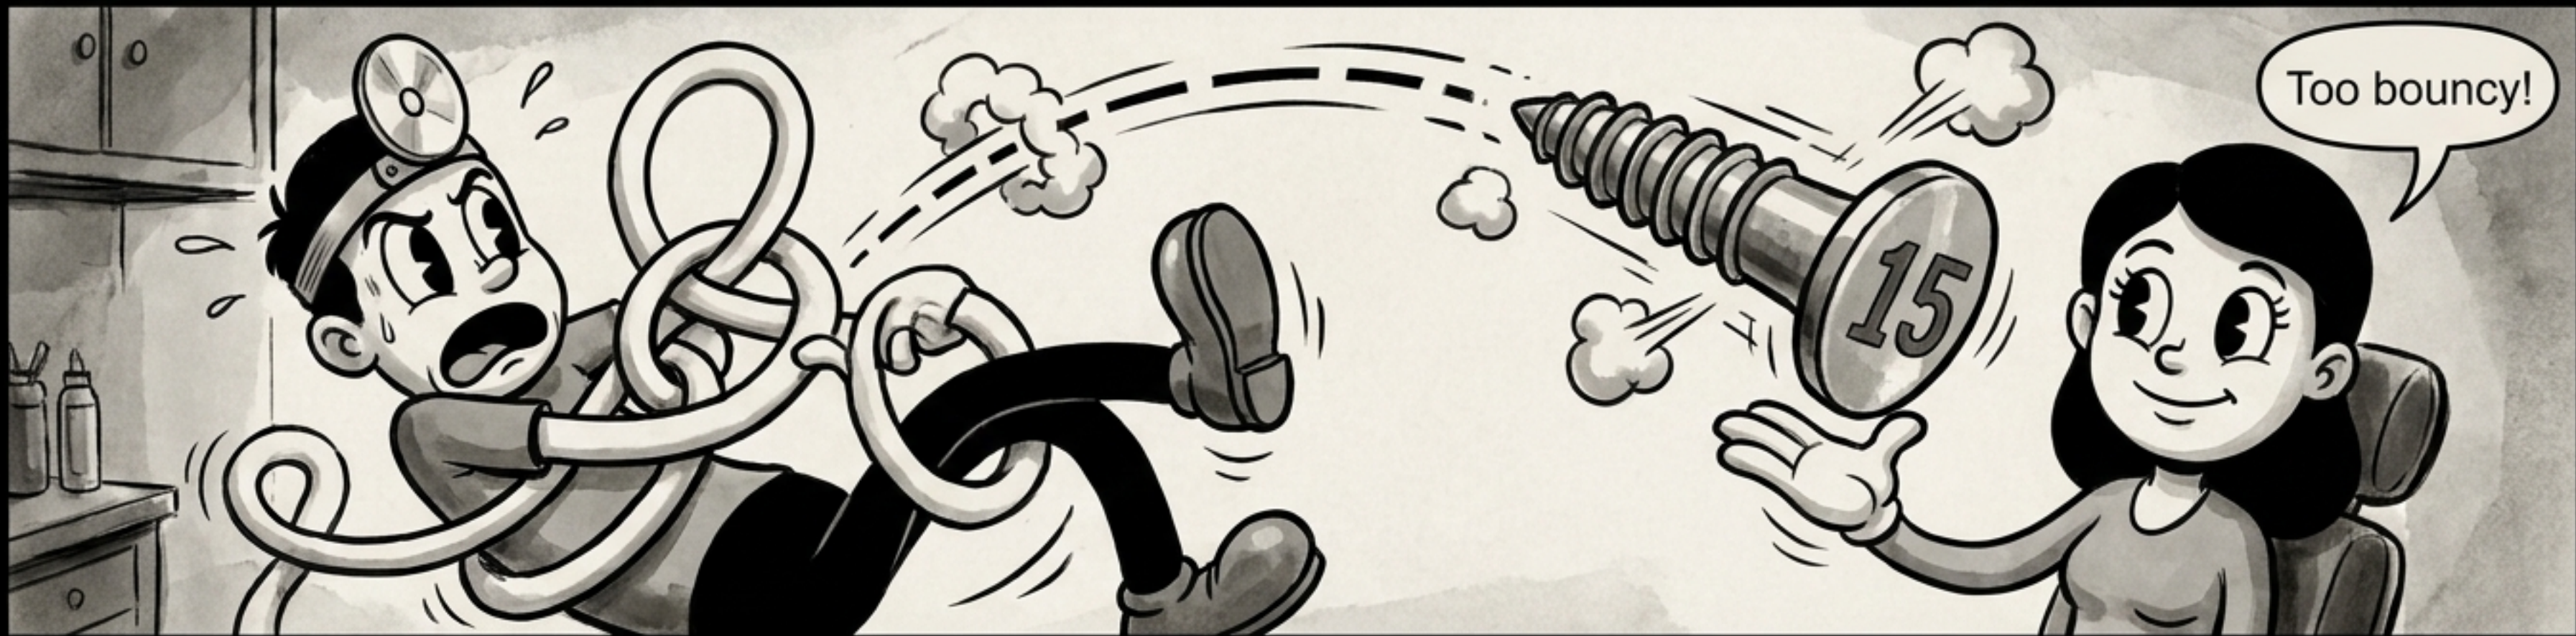

ASTM F138 implant-grade steel used for bone screws contains 13 to 15 percent nickel.
Deep tissue orthopaedics is a highly unusual aesthetic for an earlobe