Log every autoclave cycle date and time.
Record temperature, pressure, and biological indicator results.
Test autoclaves with biological indicators frequently.
Verify supplier certificates for single-use equipment.

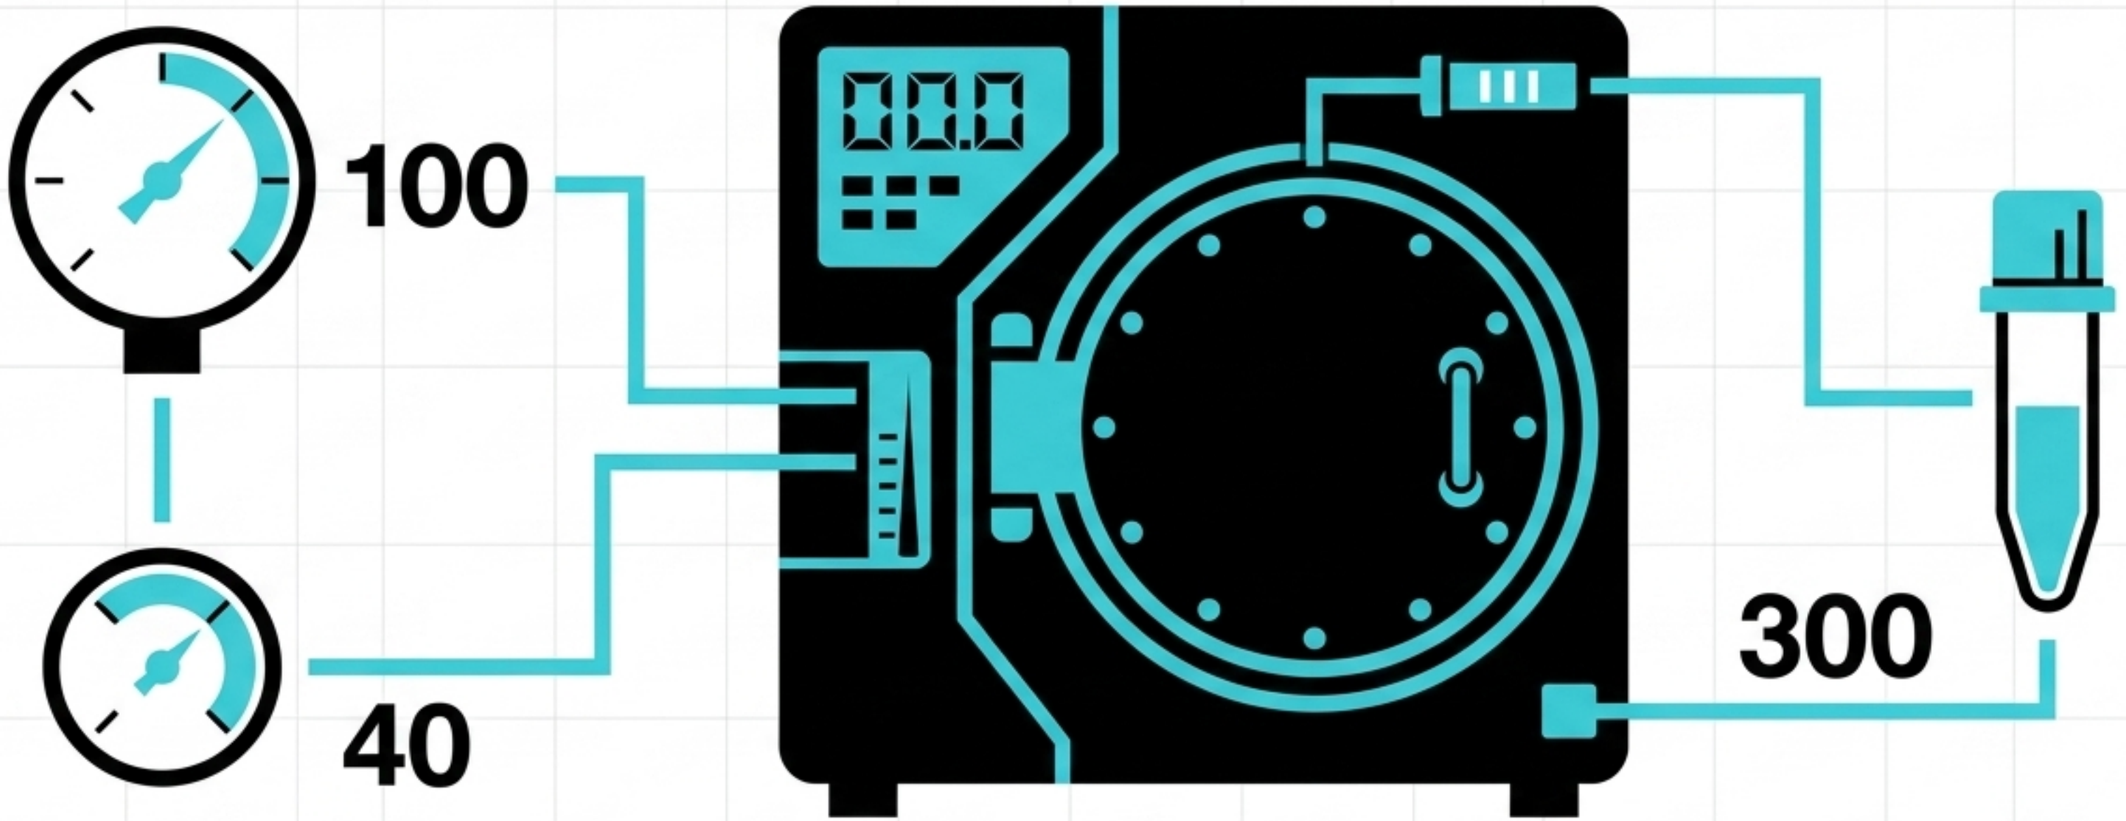

Microbial limits must remain below established cosmetic thresholds.

MAINTAIN WRITTEN STANDARD OPERATING PROCEDURES

Gemini Notebook