




Approved Implant Titanium
Select Standard F **136**

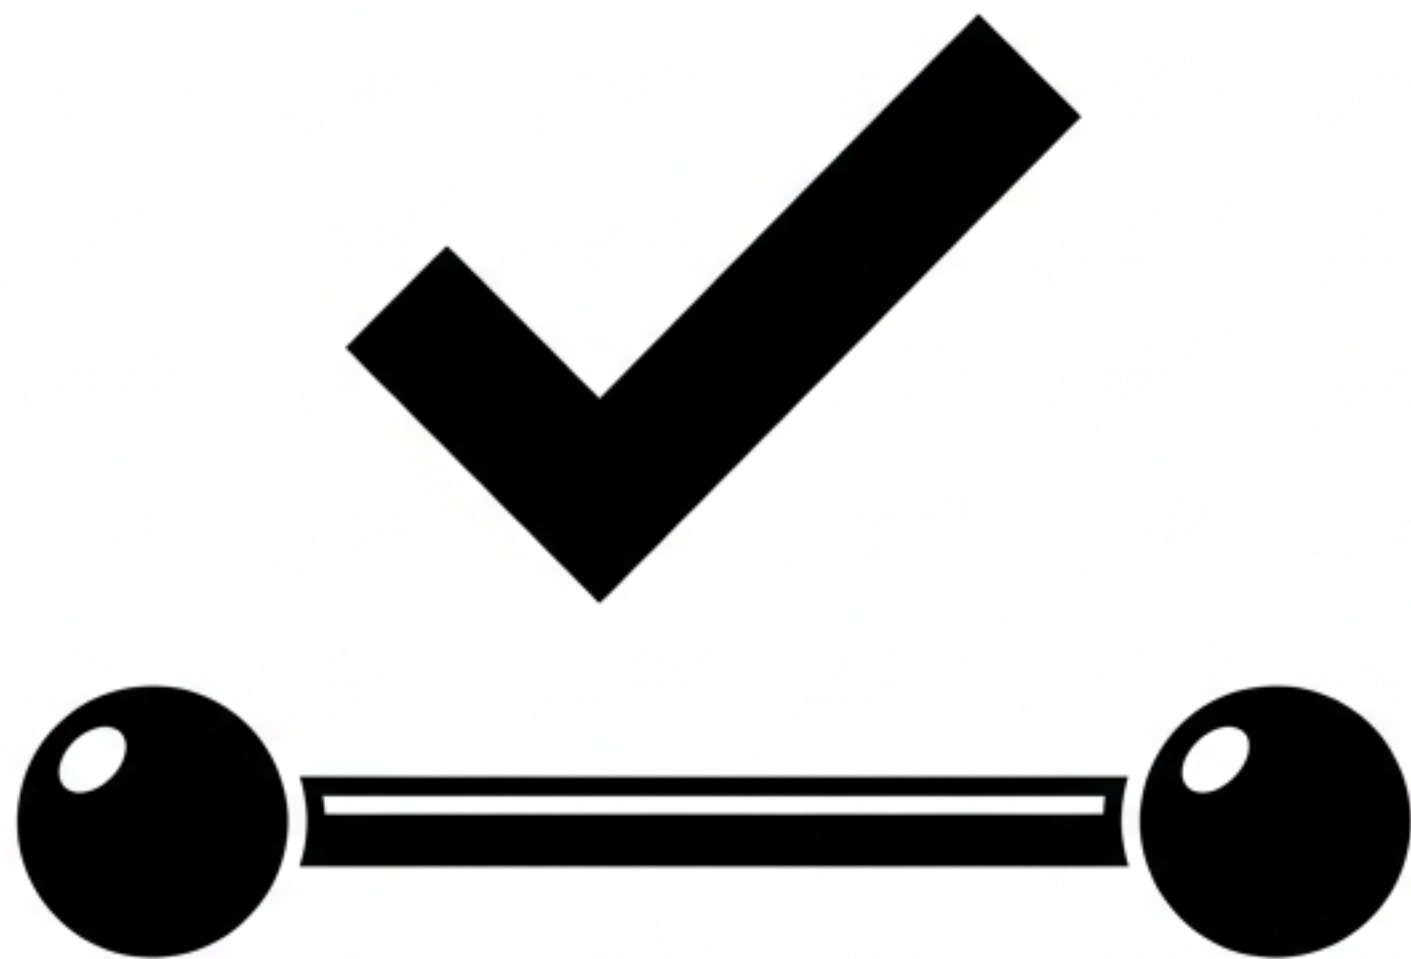

Standard Surgical Steel
Avoid During Healing Phase
10 15

This steel relies on a passive layer to limit release.

Select certified titanium for fresh tissue.