
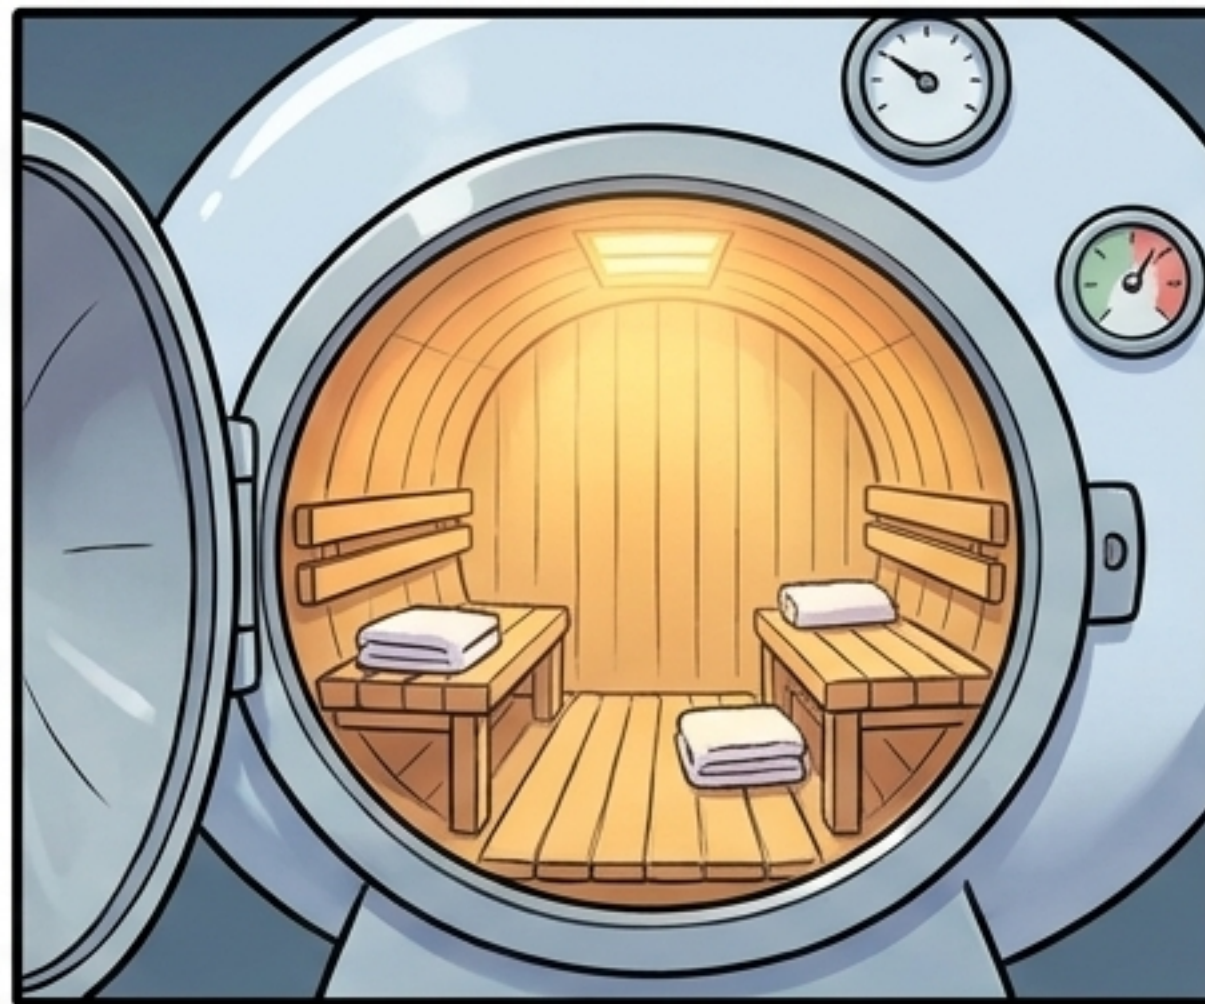


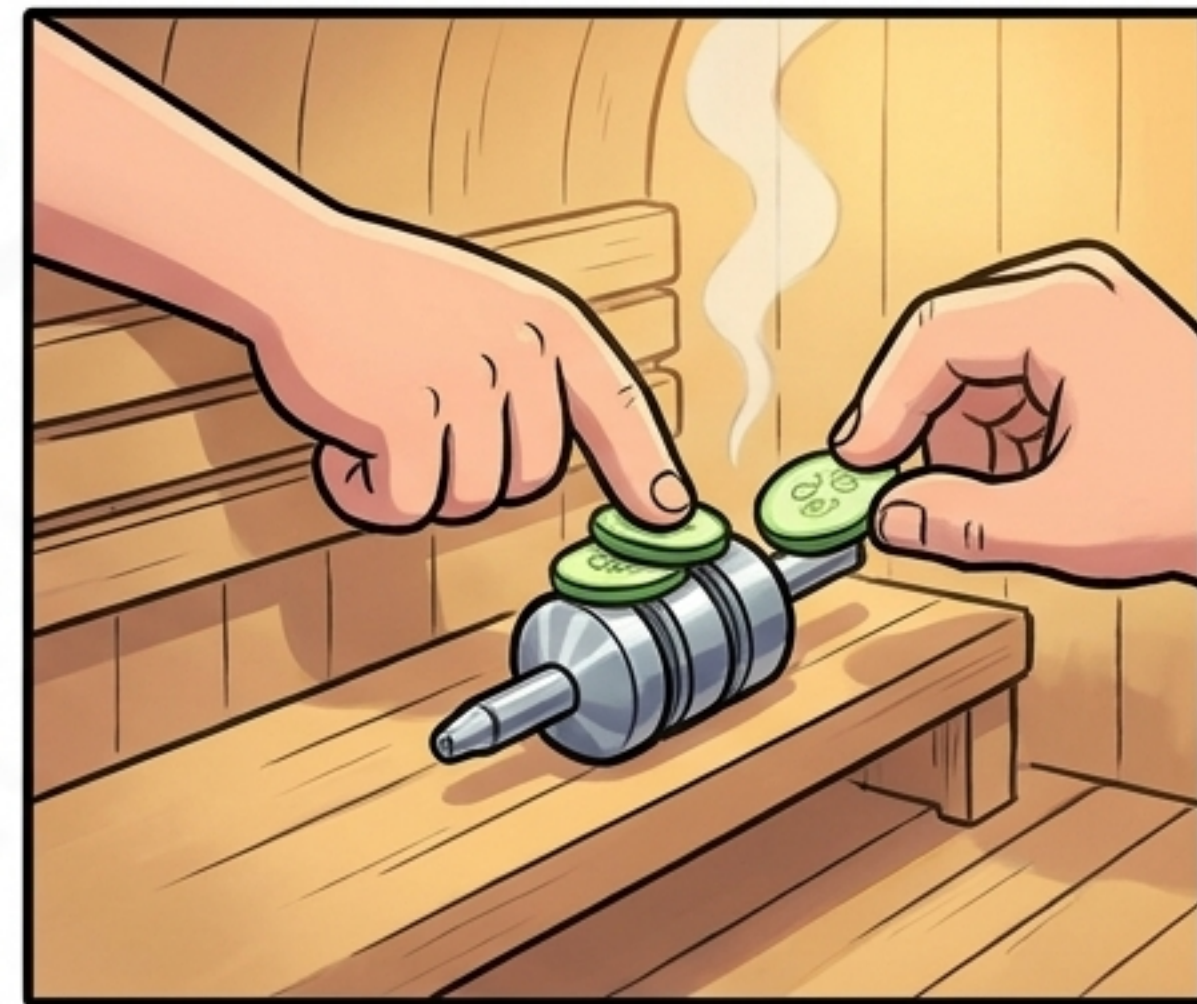

Reusable equipment must be sterilized in a regularly calibrated autoclave. Even stainless steel grips deserve a relaxing steam.