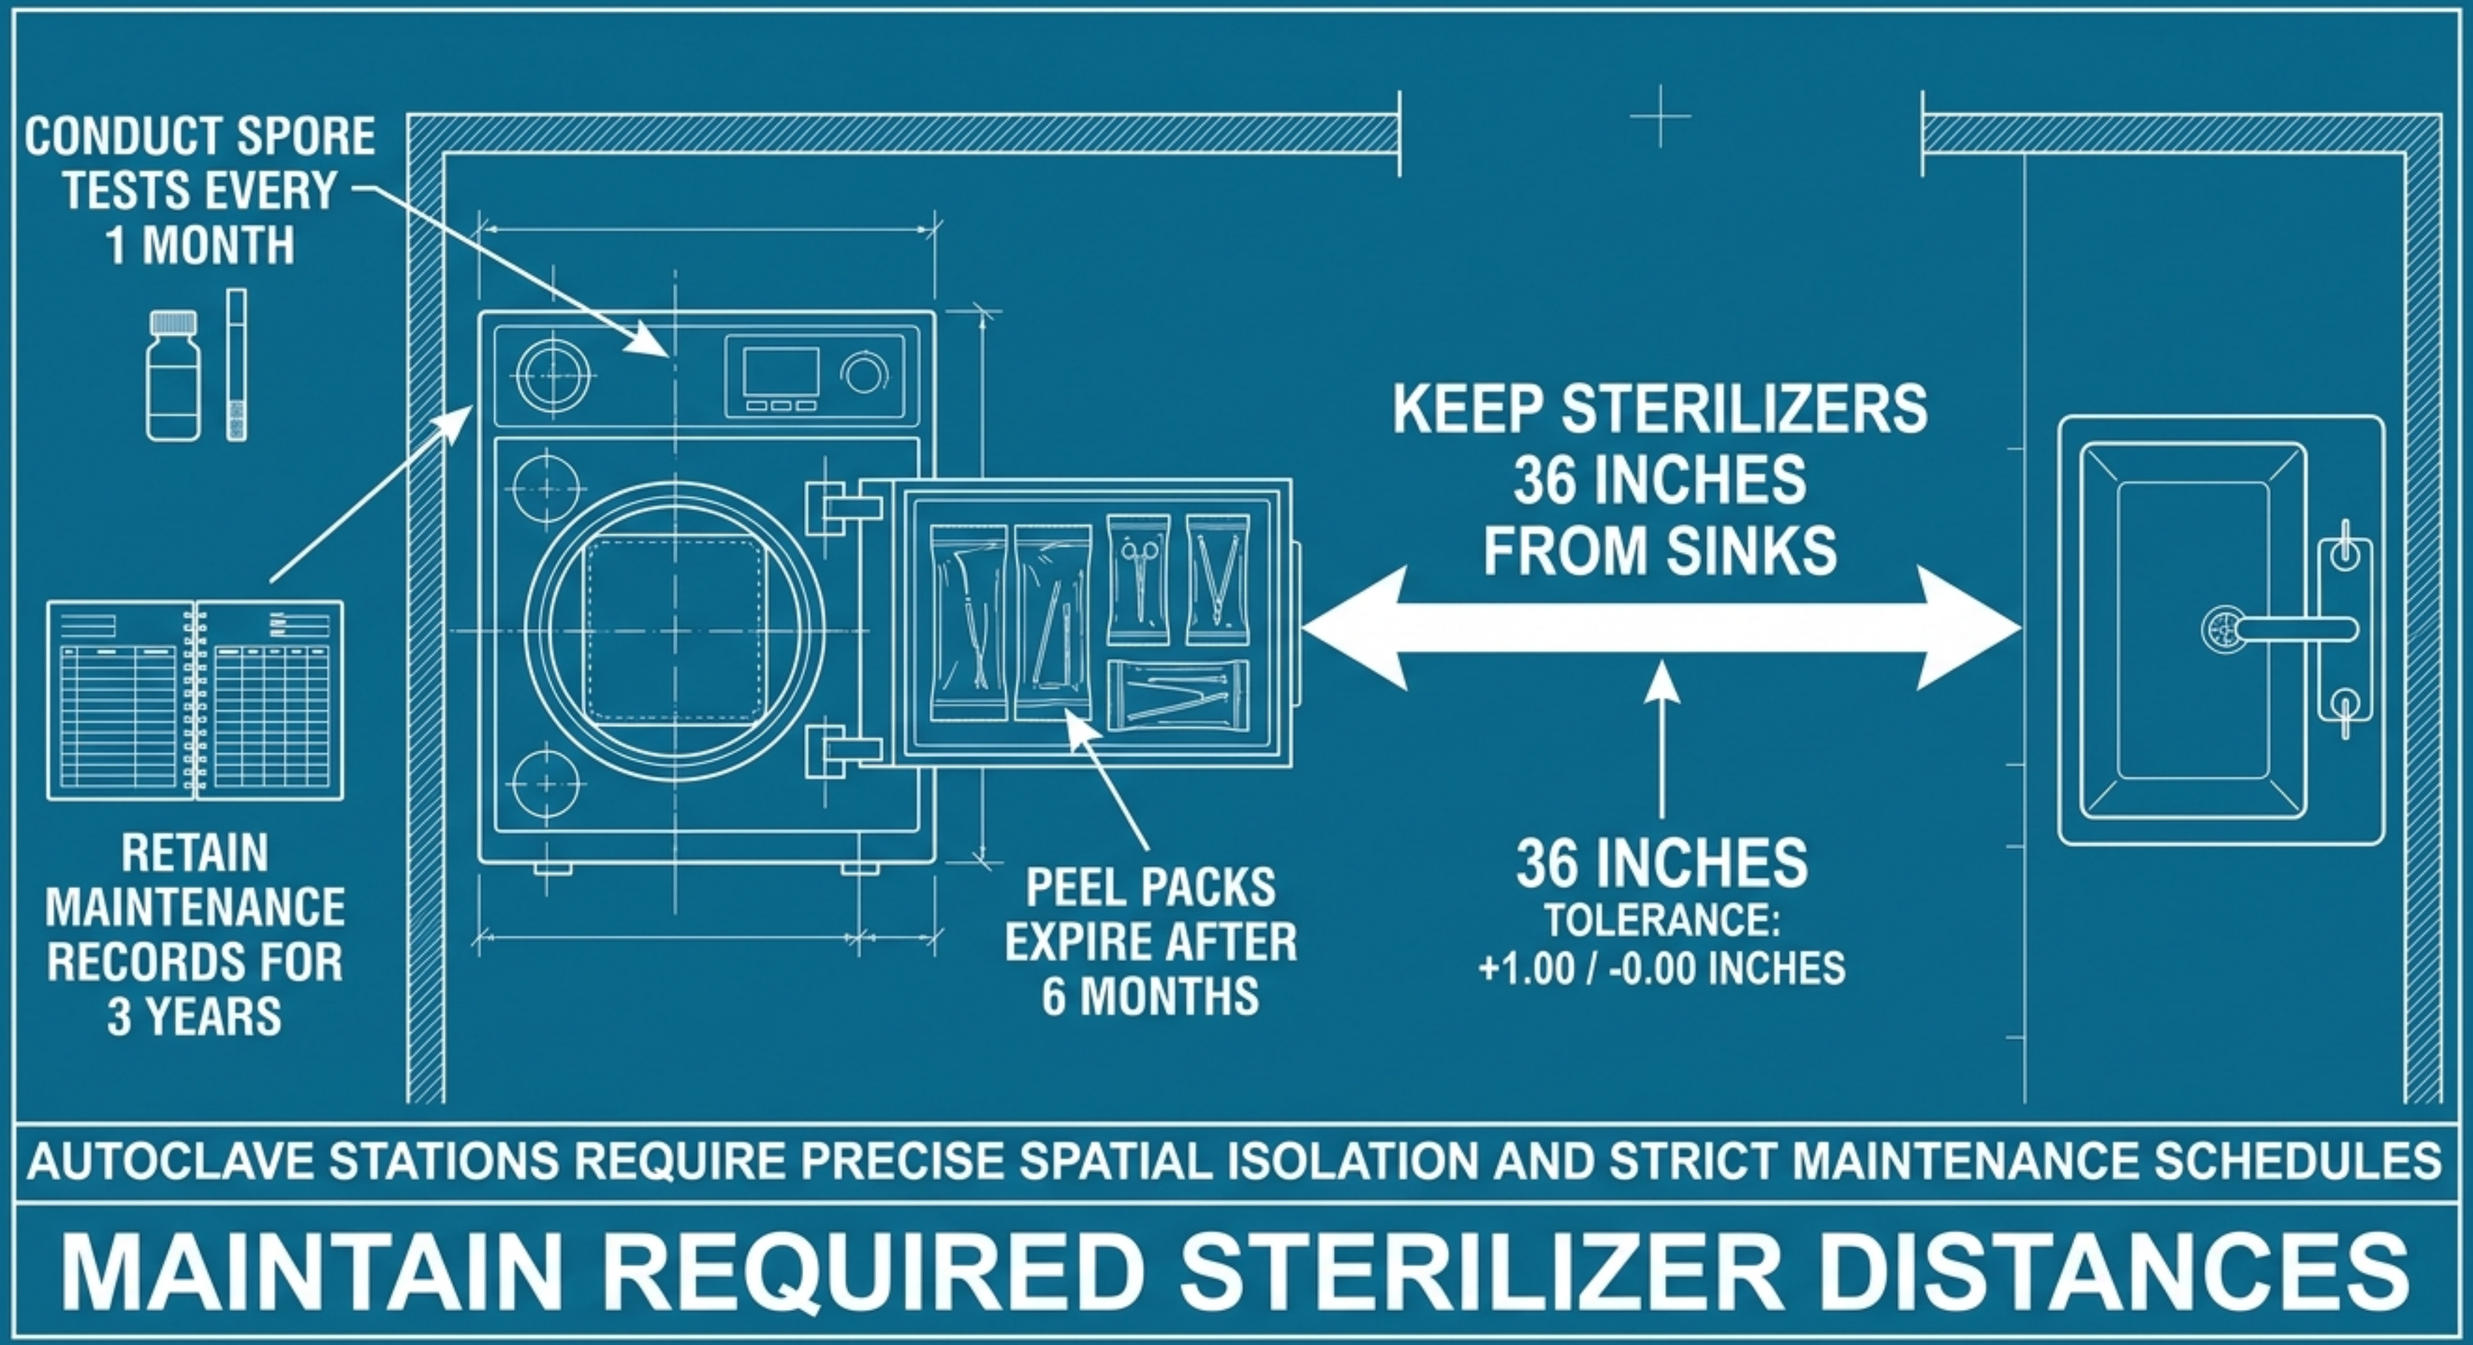

AUTOCLAVE STATIONS REQUIRE PRECISE SPATIAL ISOLATION AND STRICT MAINTENANCE SCHEDULES

MAINTAIN REQUIRED STERILIZER DISTANCES