




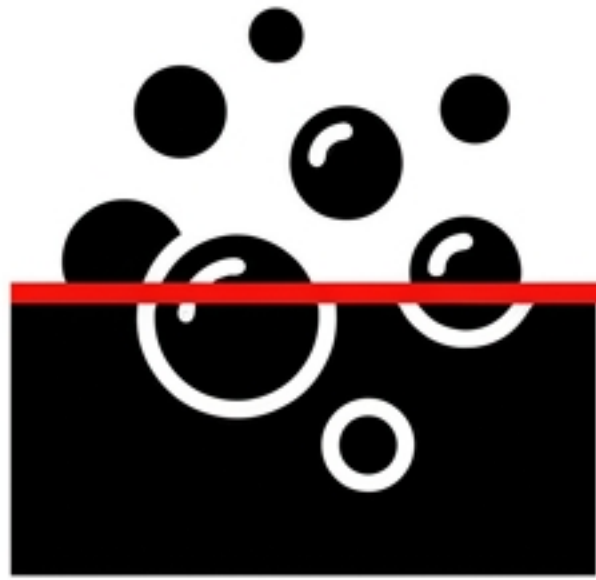

Wash items
items
manually
using soap.

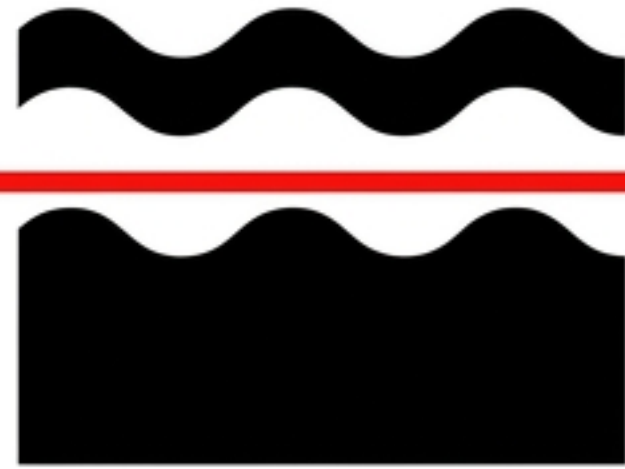

Rinse
thoroughly
thoroughly
with clean
water.

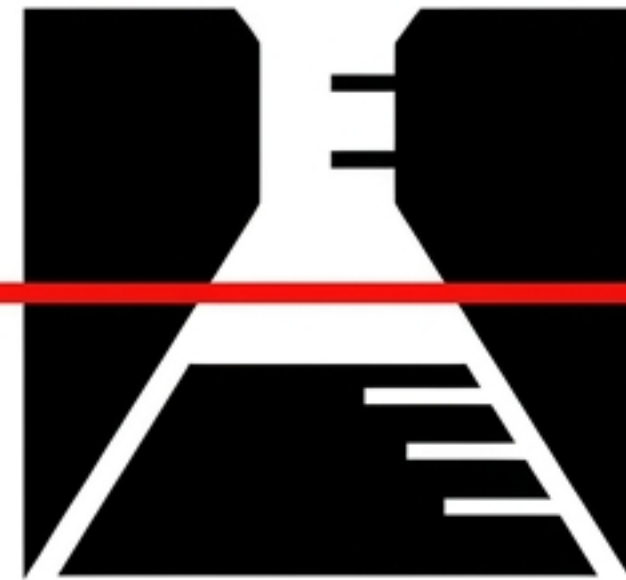

Immerse
completely
completely
in chemical
disinfectant.



Process
inside an
approved
autoclave.

Reusable instruments must undergo strict multi-stage decontamination before packaging.
FOLLOW STRICT DECONTAMINATION PROTOCOLS.