


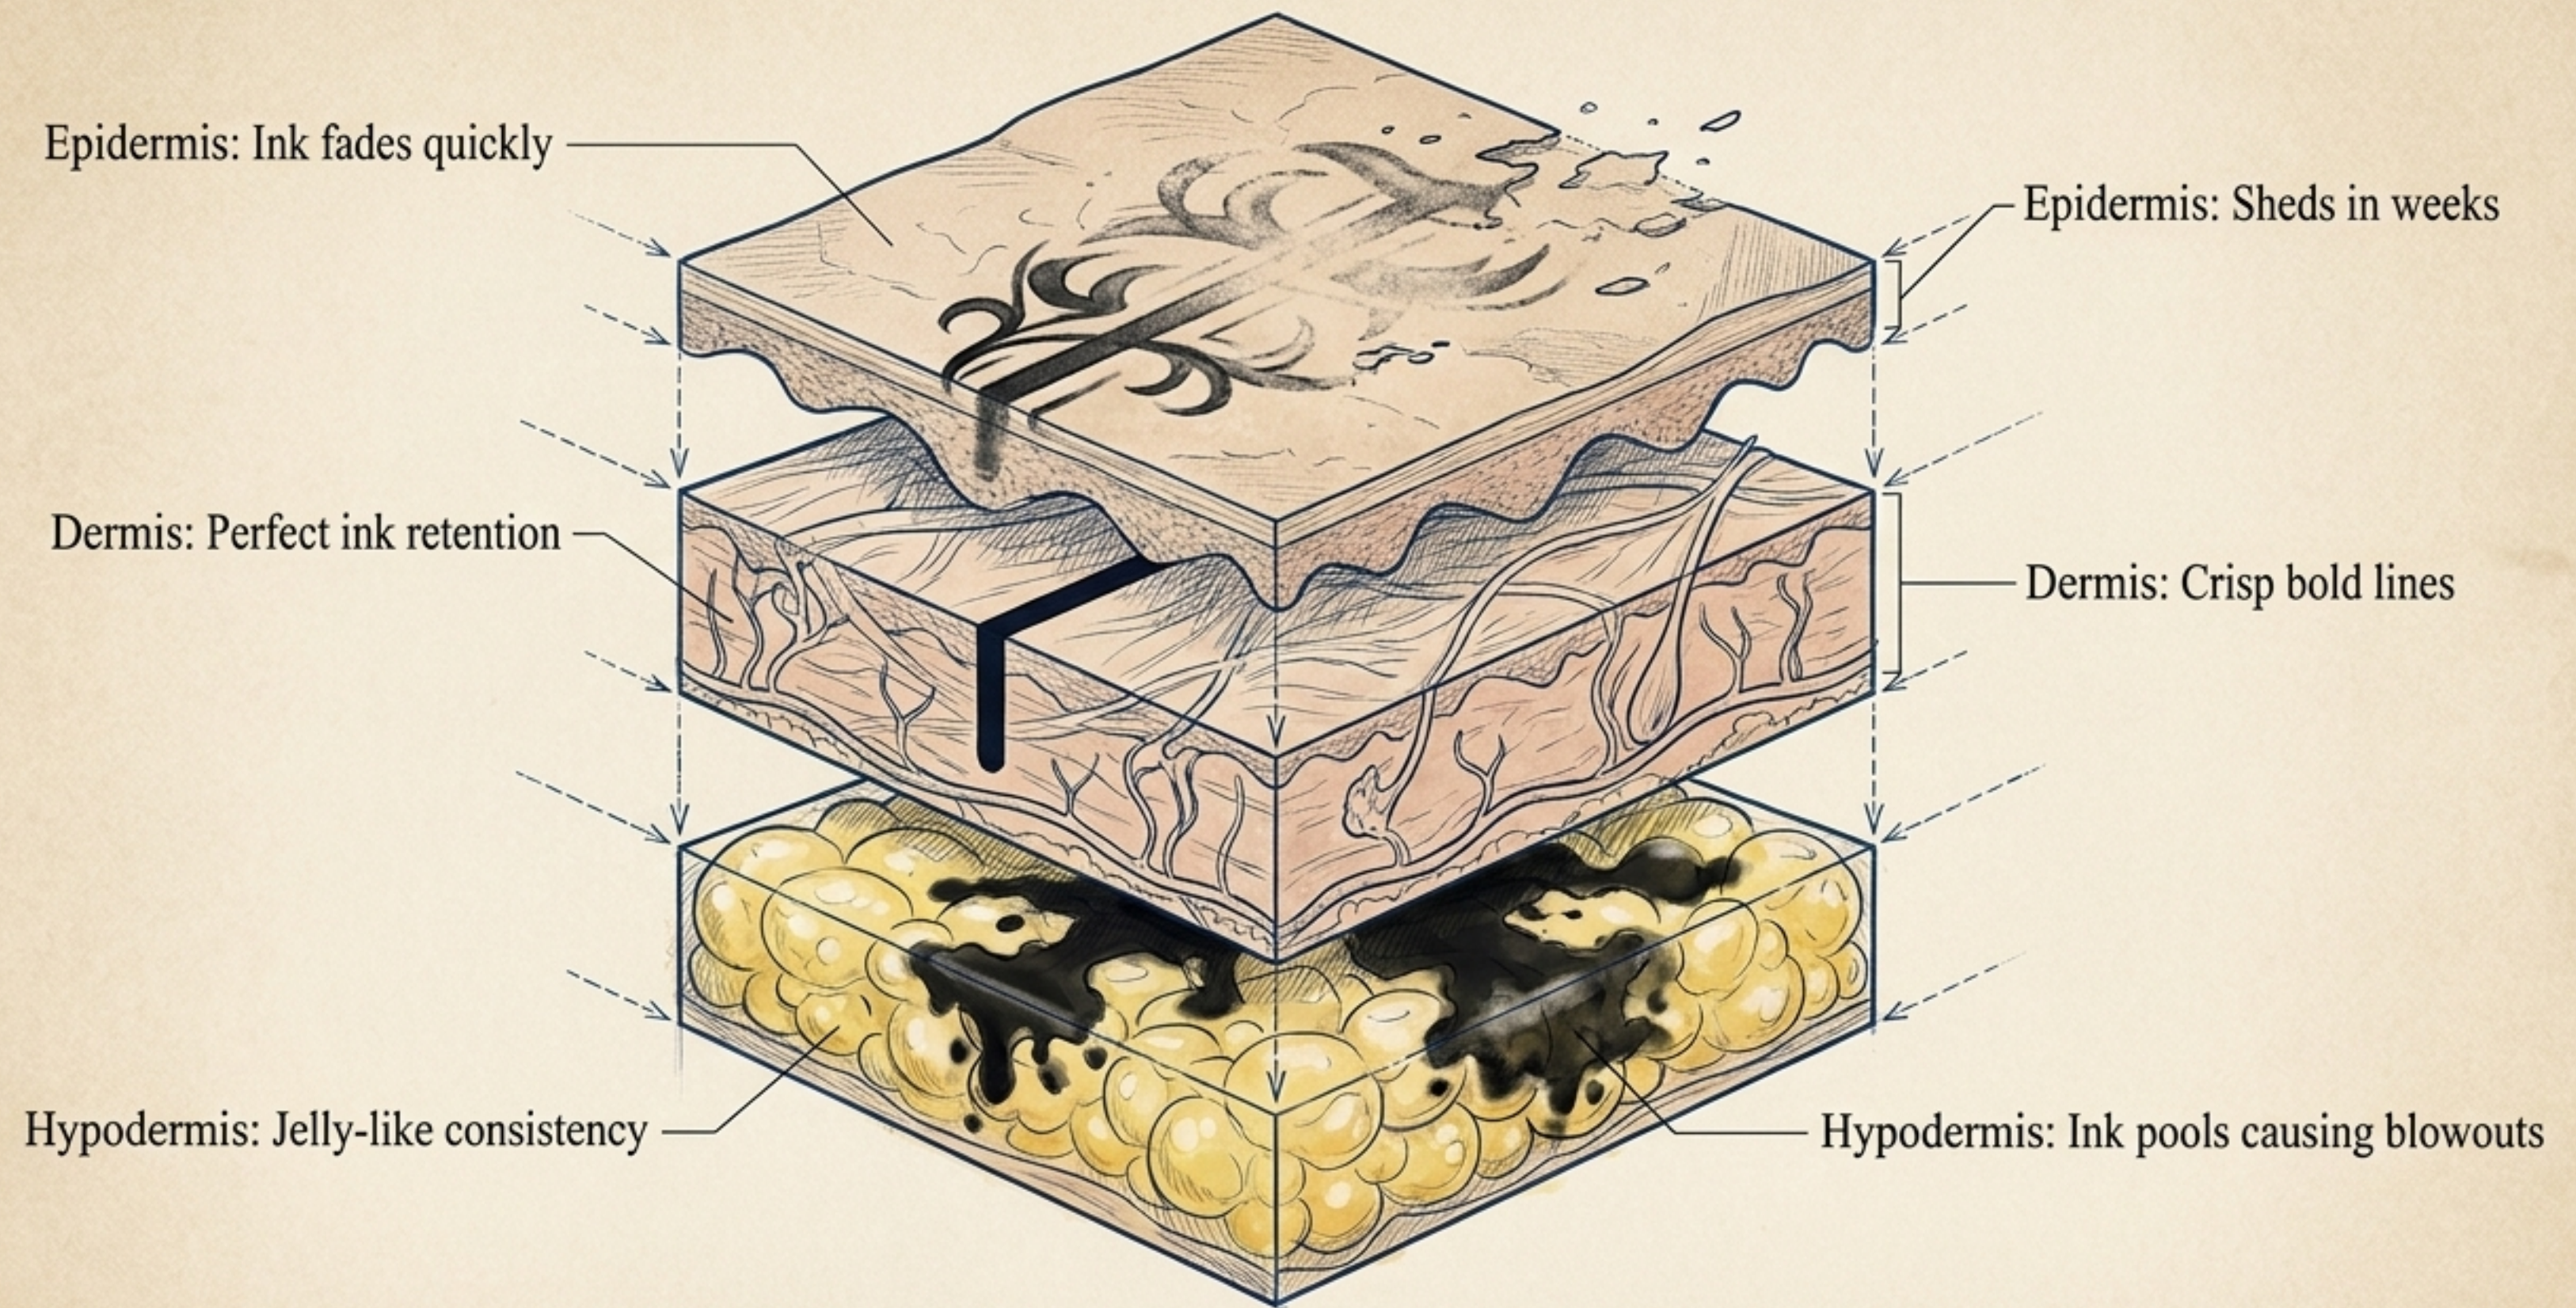

Incorrect needle calibration results in rapid fading at the surface or severe blowouts in the fat layer.

MASTERING THE DERMAL TARGET