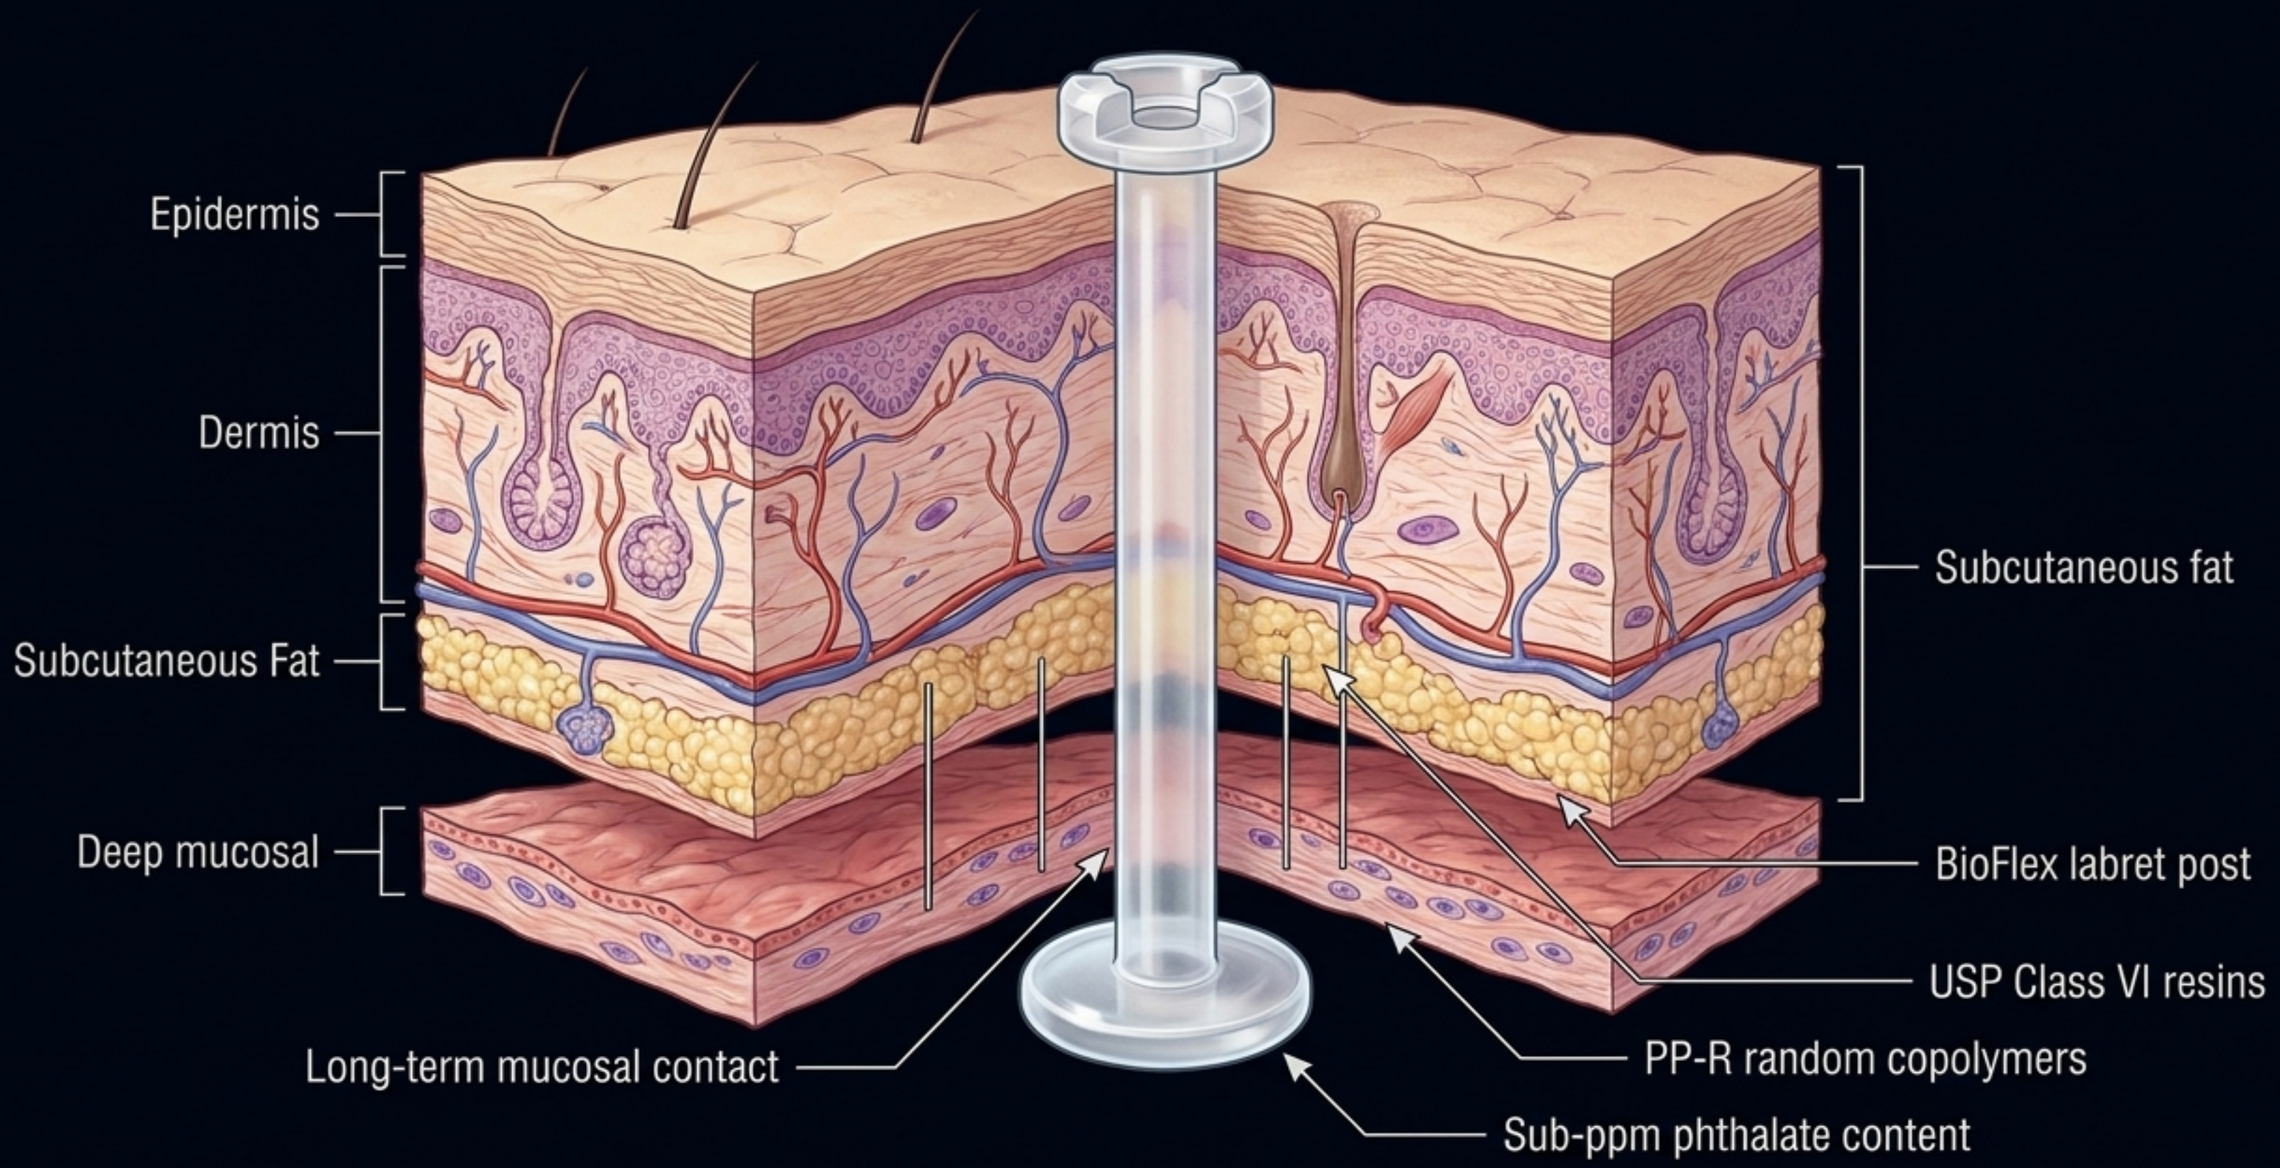

Hardware designed for mucosal contact relies on certified polymers with sub-ppm phthalates.

BIOCOMPATIBILITY AND HARDWARE IMPLANTATION

Gemini Notebook