



Use **implant grade titanium ASTM 136**.
Solid **14 or 18 karat gold** is safe.

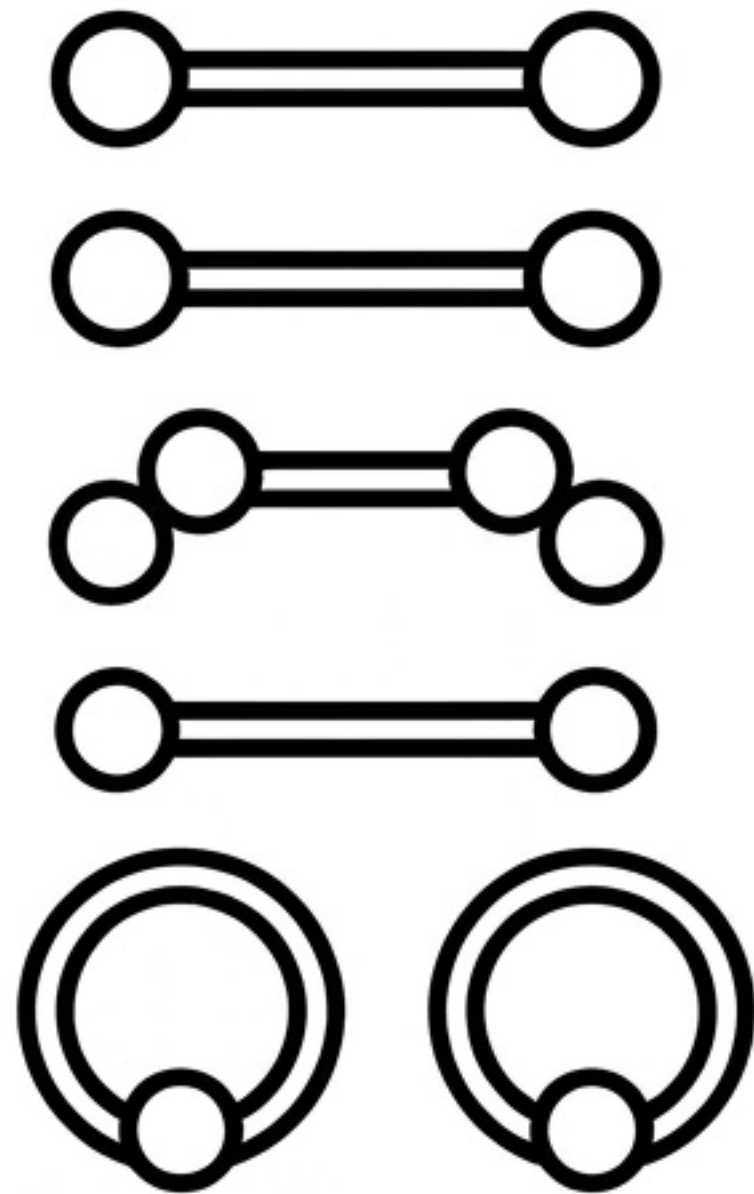

Do not use **plated mystery metals**.
Avoid **surgical steel** and **sterling silver**.

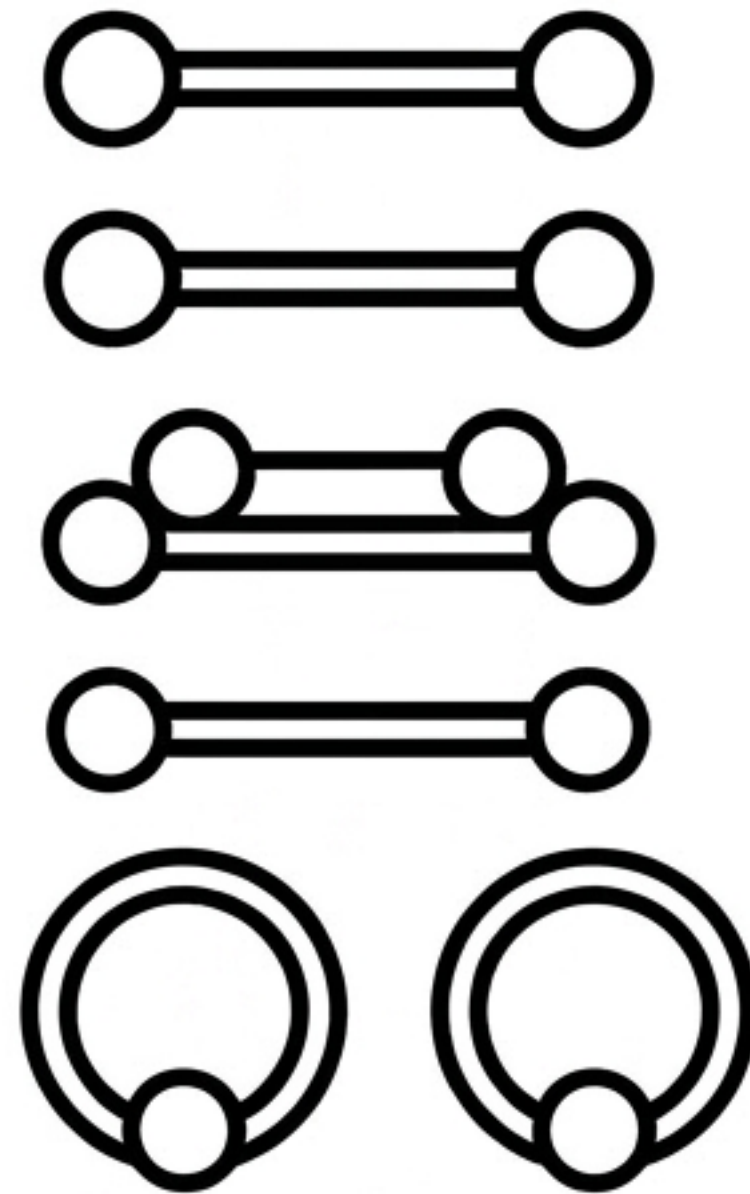

Biocompatible metals prevent immune system rejection.
Never use cheap metals for healing.